
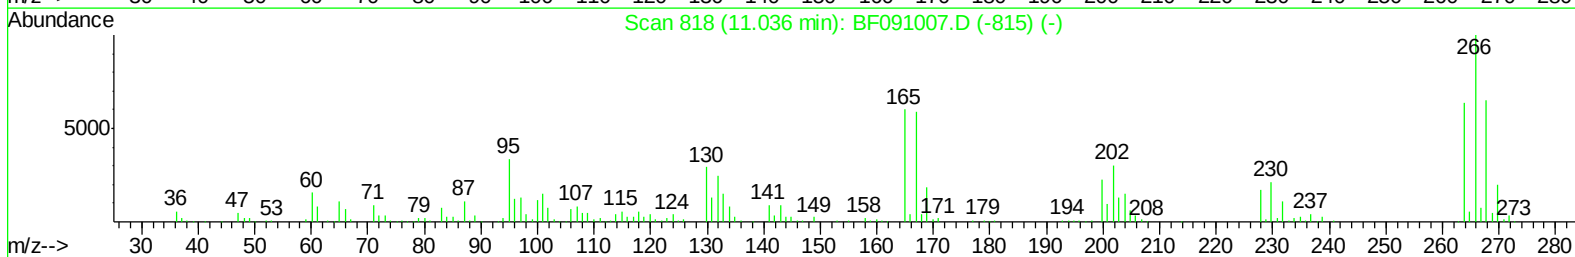
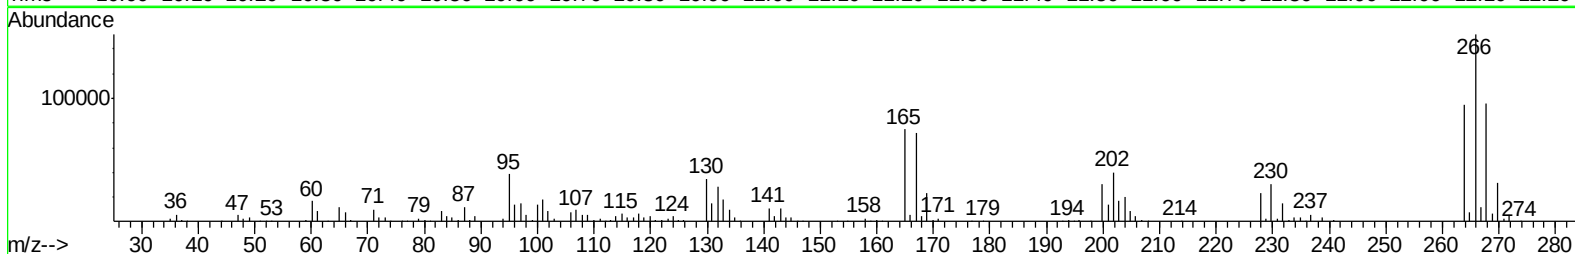


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110316\
Data File : BF091003.D
Acq On : 3 Nov 2016 17:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:49:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 01:48:09 2016
Response via : Initial Calibration

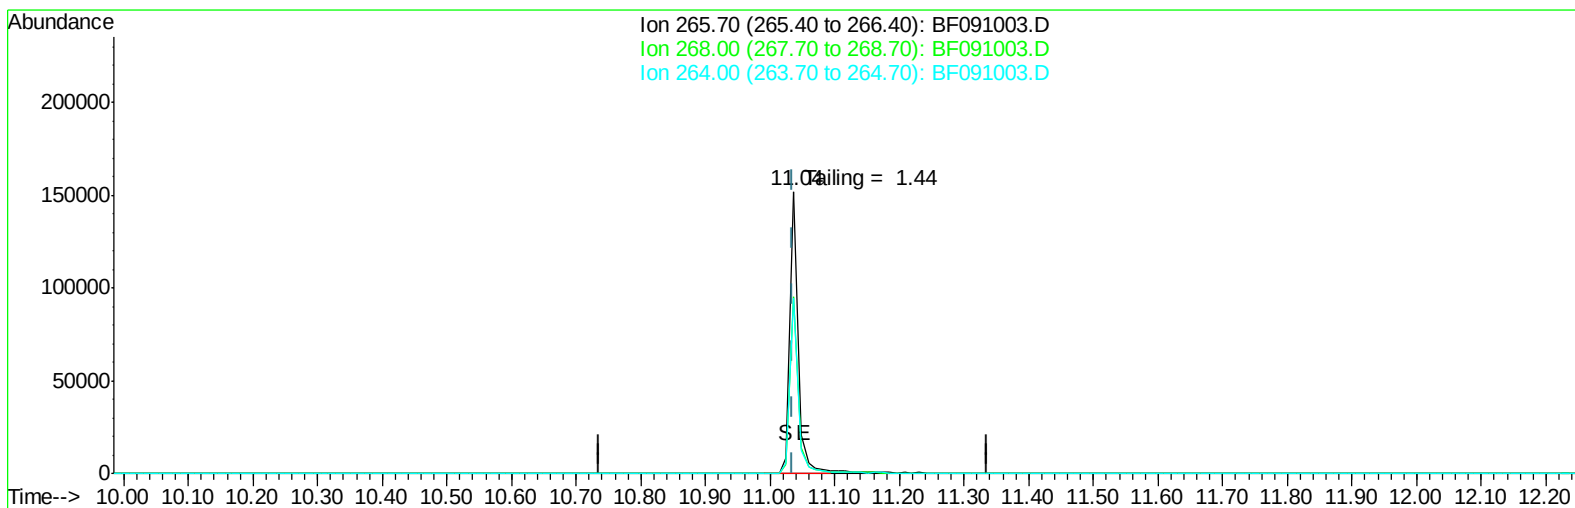

TIC: BF091003.D

(69) Pentachlorophenol (C)




11.036min (+0.000) 0.00ng

response 138097

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.81
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110316\
Data File : BF091003.D
Acq On : 3 Nov 2016 17:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:49:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 01:48:09 2016
Response via : Initial Calibration

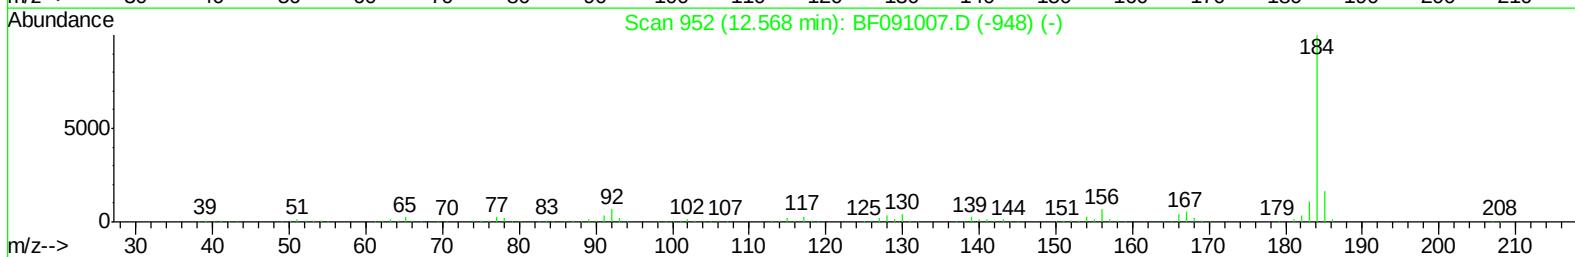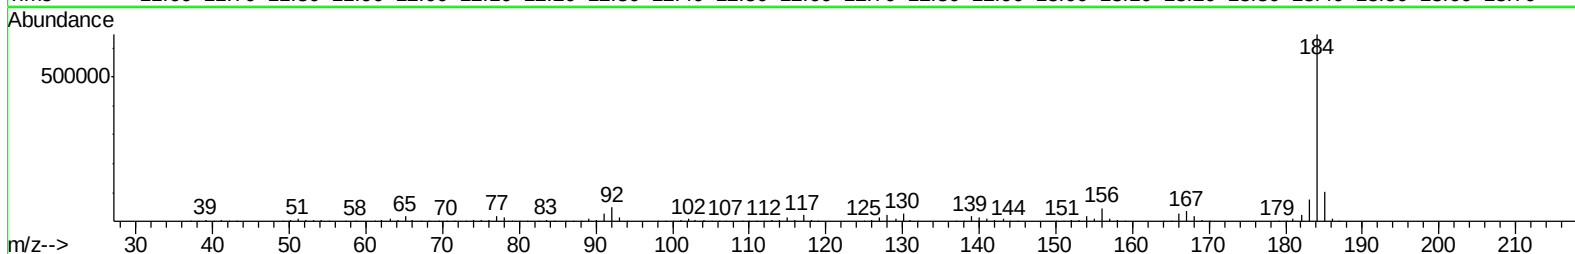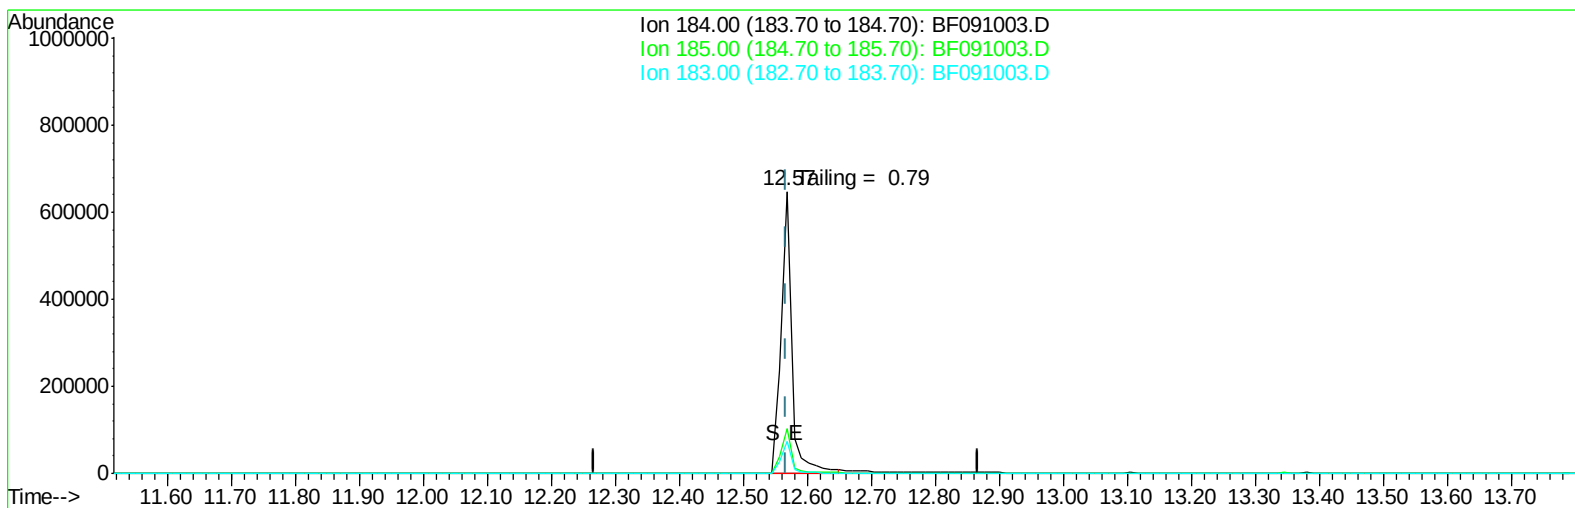

TIC: BF091003.D

(76) Benzidine

12.568min (+0.000) 0.00ng

response 774401

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.95
183.00	10.90	11.58
0.00	0.00	0.00