


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF110316\  
 Data File : BF091003.D  
 Acq On : 3 Nov 2016 17:57  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110316.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Nov 04 11:03:12 2016

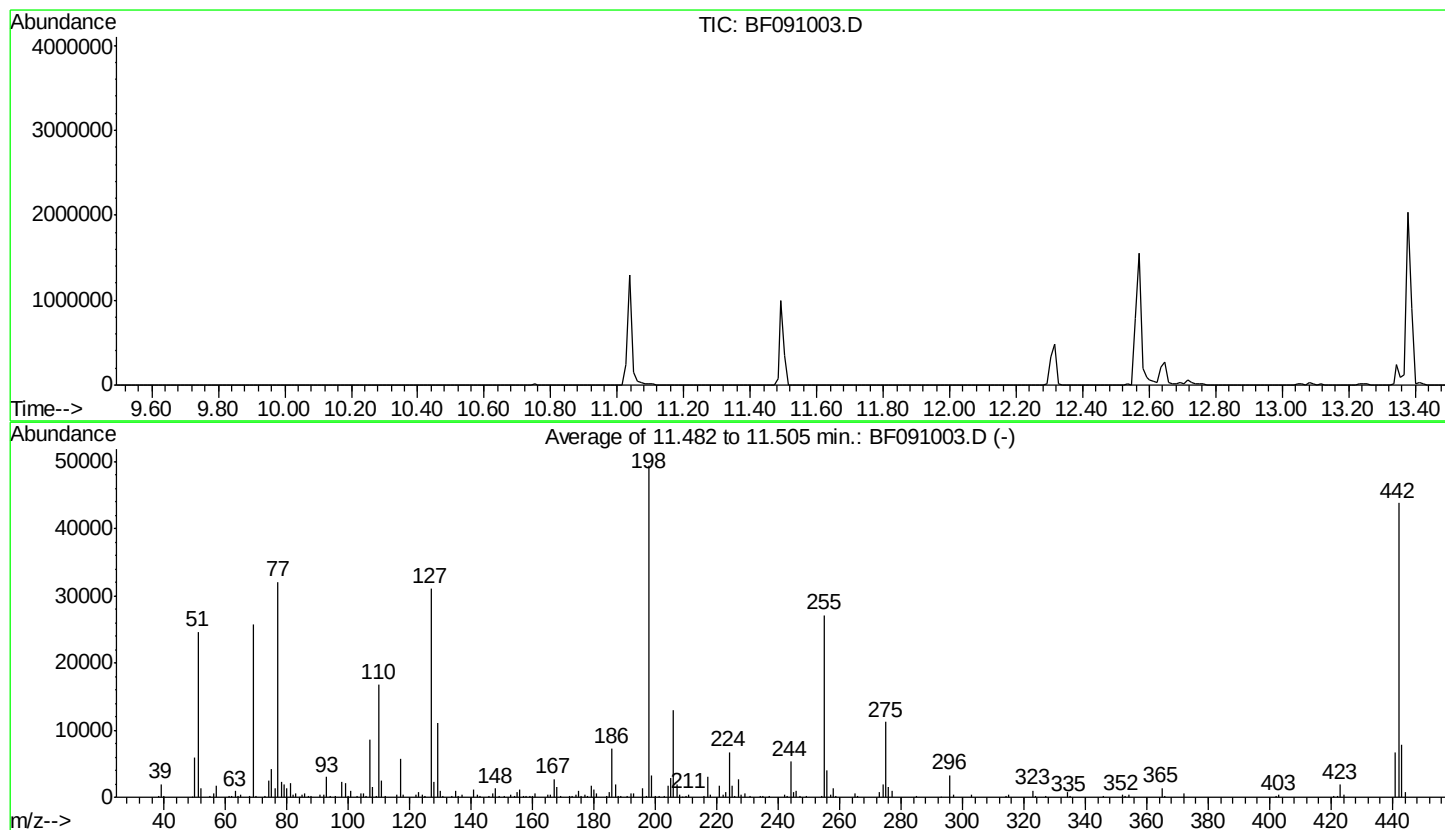

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 49.9      | 24633   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 269     | PASS             |
| 69          | 198          | 0.00         | 100          | 52.3      | 25839   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 147     | PASS             |
| 127         | 198          | 10           | 80           | 62.8      | 30999   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 109     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 49399   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 3294    | PASS             |
| 275         | 198          | 10           | 60           | 22.7      | 11232   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 1349    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.4      | 6747    | PASS             |
| 442         | 198          | 50           | 100          | 88.8      | 43850   | PASS             |
| 443         | 442          | 15           | 24           | 17.9      | 7836    | PASS             |