


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110317\
 Data File : BF100130.D
 Acq On : 3 Nov 2017 12:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 03 15:46:10 2017

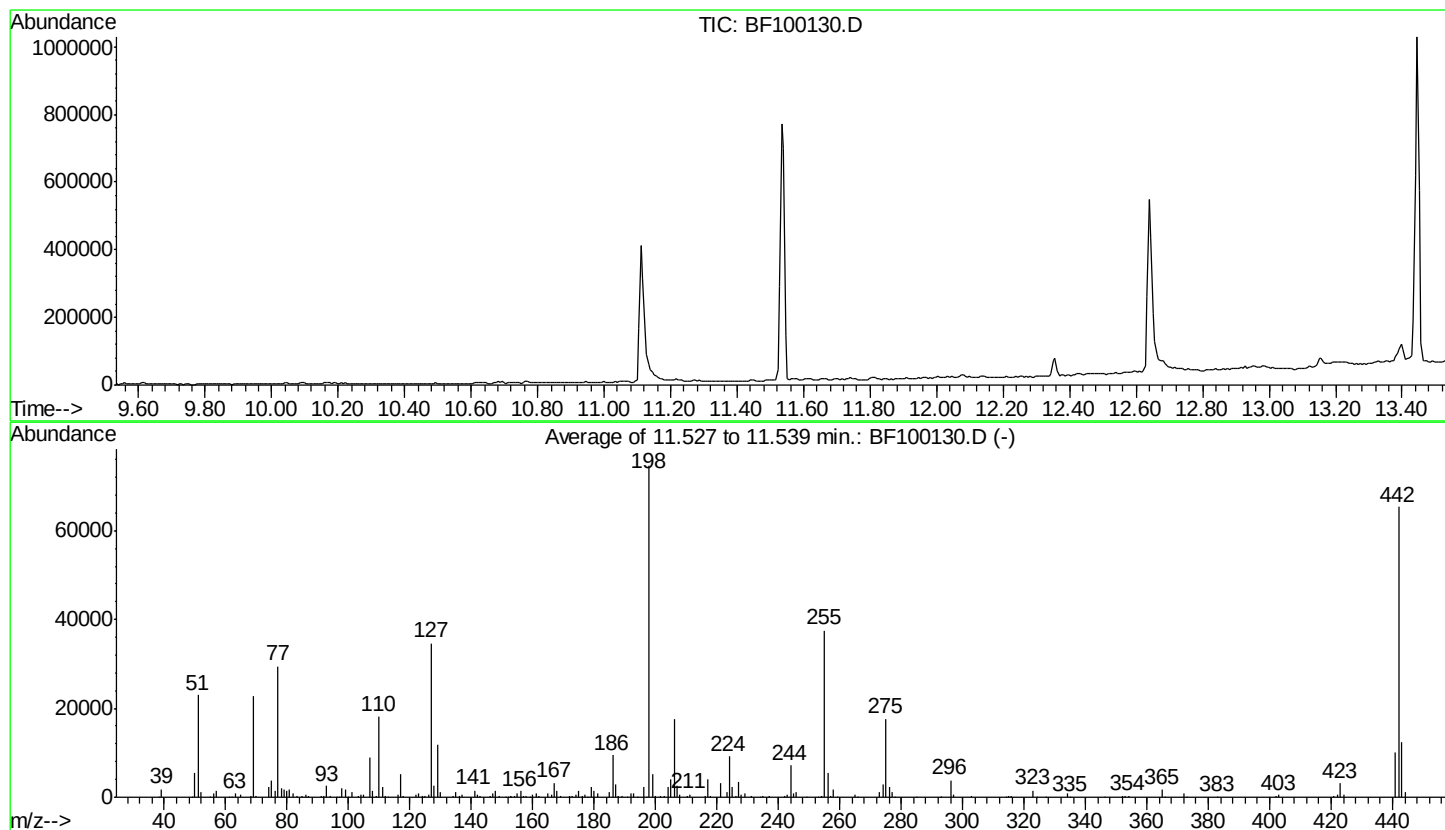

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	22978	PASS
68	69	0.00	2	1.8	418	PASS
69	198	0.00	100	30.6	22800	PASS
70	69	0.00	2	0.9	208	PASS
127	198	10	80	46.5	34701	PASS
197	198	0.00	2	0.2	144	PASS
198	198	100	100	100.0	74621	PASS
199	198	5	9	6.8	5102	PASS
275	198	10	60	23.7	17691	PASS
365	198	1	100	2.3	1705	PASS
441	443	0.01	100	81.5	10021	PASS
442	198	50	100	87.5	65310	PASS
443	442	15	24	18.8	12303	PASS