
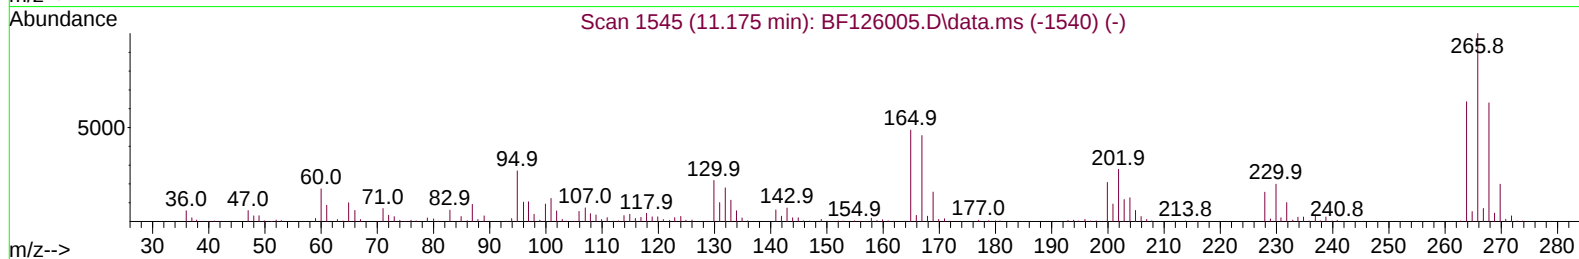
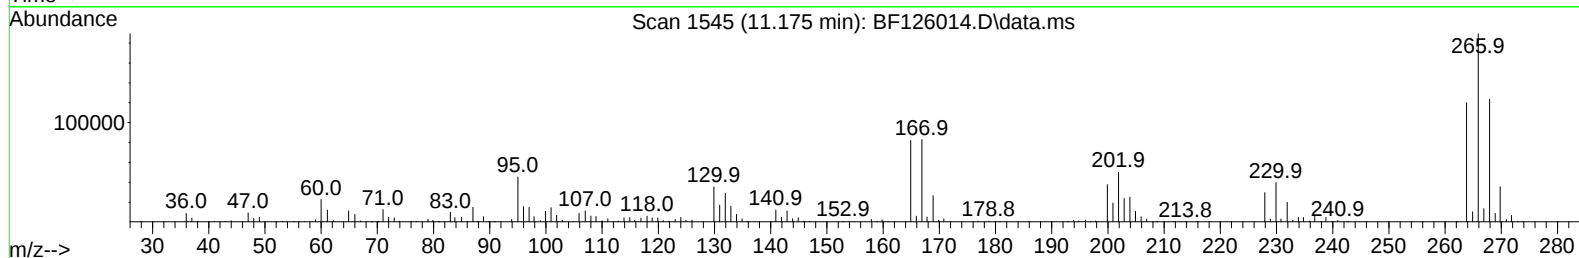


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110321\
Data File : BF126014.D
Acq On : 3 Nov 2021 11:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 16:09:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 16:05:25 2021
Response via : Initial Calibration

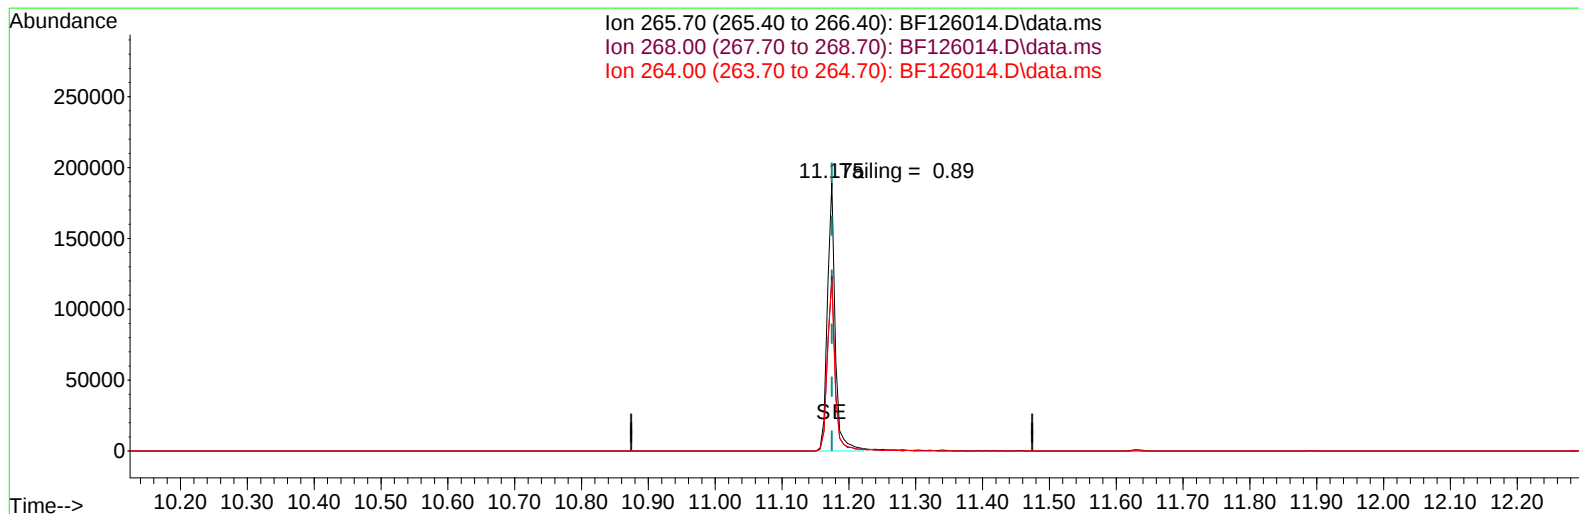

TIC: BF126014.D\data.ms

(70) Pentachlorophenol (C)




11.175min (-0.000) 24864.56 ng

response 157403

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.24
264.00	69.90	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110321\
 Data File : BF126014.D
 Acq On : 3 Nov 2021 11:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 16:09:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 16:05:25 2021
 Response via : Initial Calibration

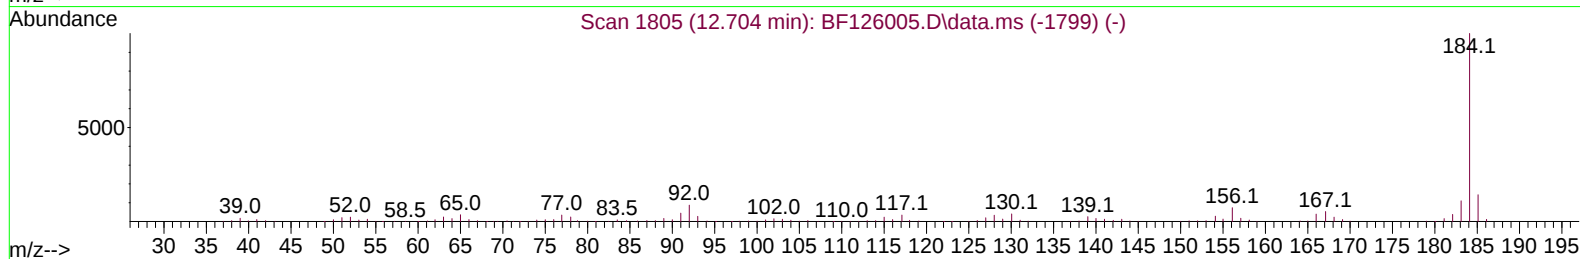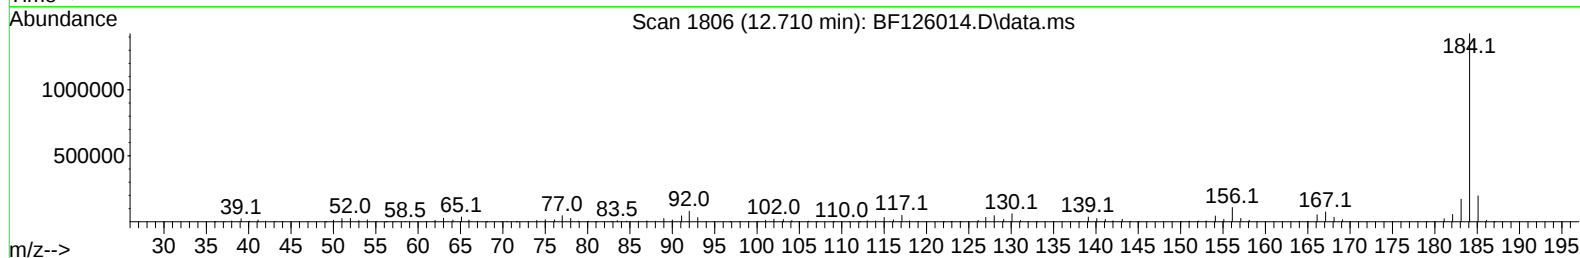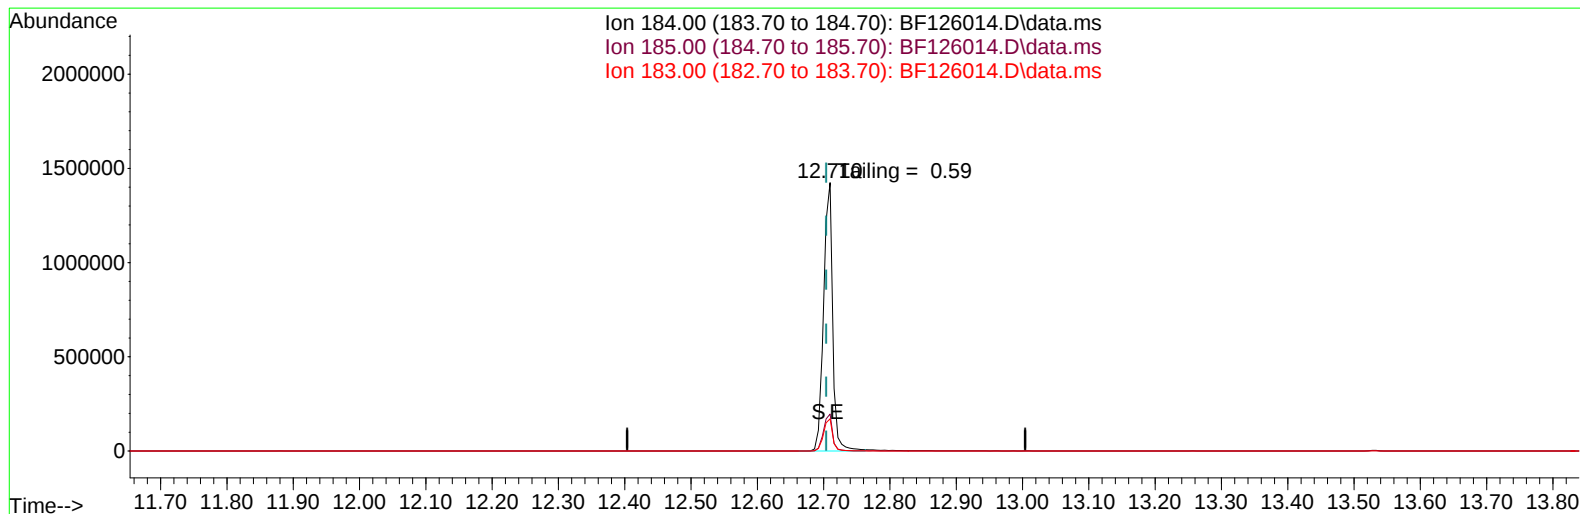

TIC: BF126014.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1362034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.81
183.00	10.10	12.00
0.00	0.00	0.00