


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110321\
 Data File : BF126014.D
 Acq On : 3 Nov 2021 11:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 03 17:21:25 2021

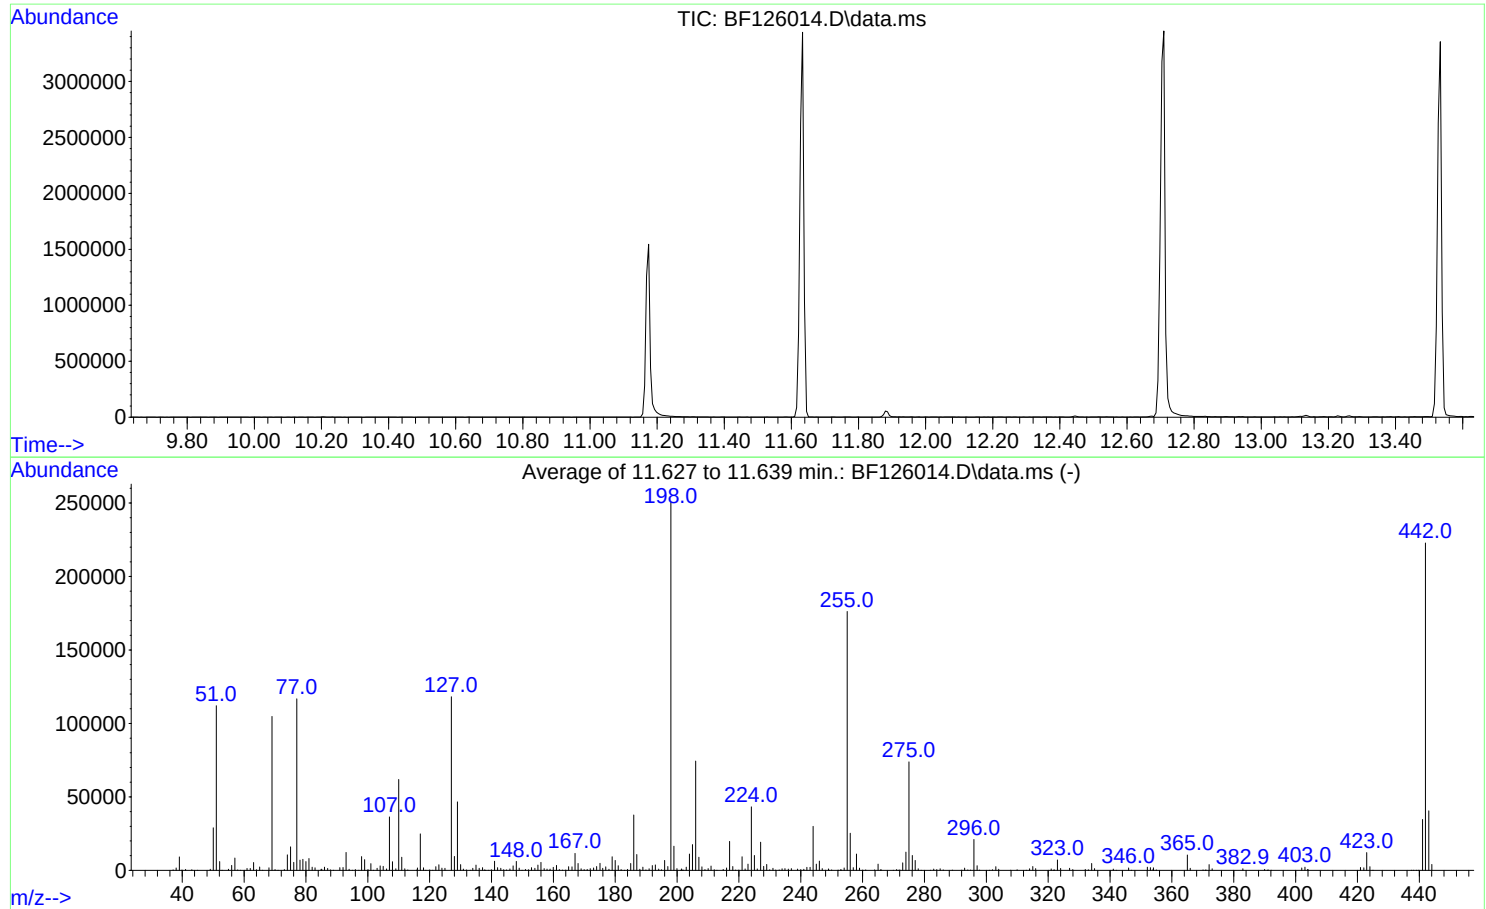




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	112040	PASS
68	69	0.00	2	1.7	1750	PASS
69	198	0.00	100	41.9	104789	PASS
70	69	0.00	2	0.5	512	PASS
127	198	10	80	47.2	118189	PASS
197	198	0.00	2	1.0	2593	PASS
198	198	100	100	100.0	250357	PASS
199	198	5	9	6.6	16445	PASS
275	198	10	60	29.5	73861	PASS
365	198	1	100	4.2	10429	PASS
441	198	0.01	100	13.8	34627	PASS
442	442	50	100	100.0	222805	PASS
443	442	15	24	18.2	40488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110321\
Data File : BF126014.D
Acq On : 3 Nov 2021 11:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 03 16:09:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 16:05:25 2021
Response via : Initial Calibration

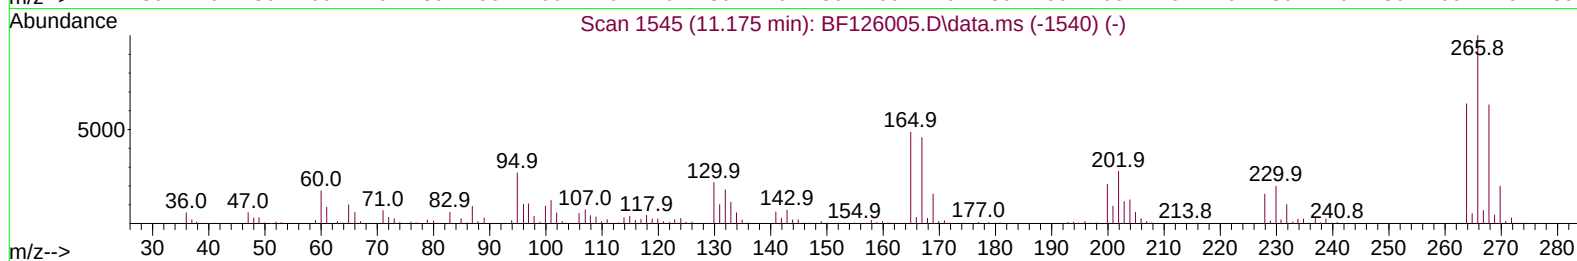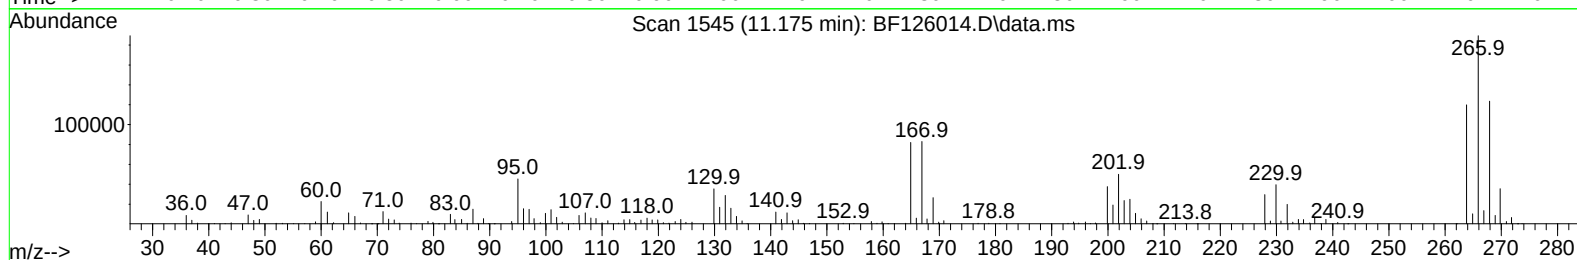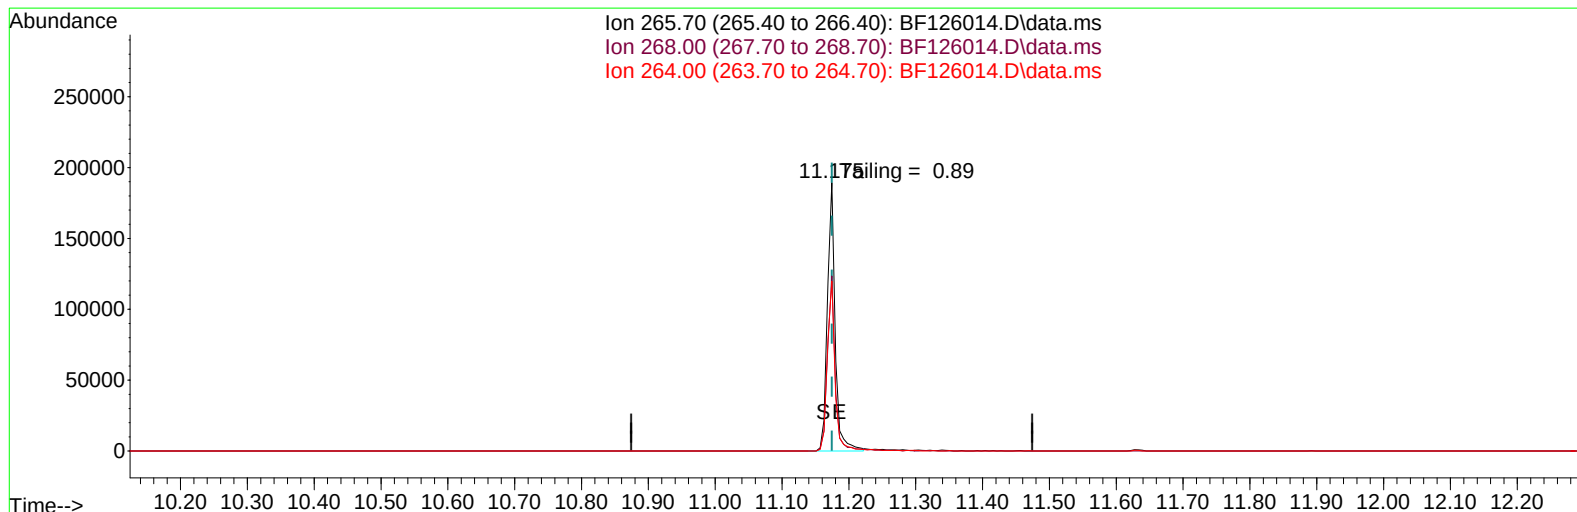

TIC: BF126014.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 24864.56 ng




response 157403

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.24
264.00	69.90	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110321\
 Data File : BF126014.D
 Acq On : 3 Nov 2021 11:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 16:09:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 16:05:25 2021
 Response via : Initial Calibration

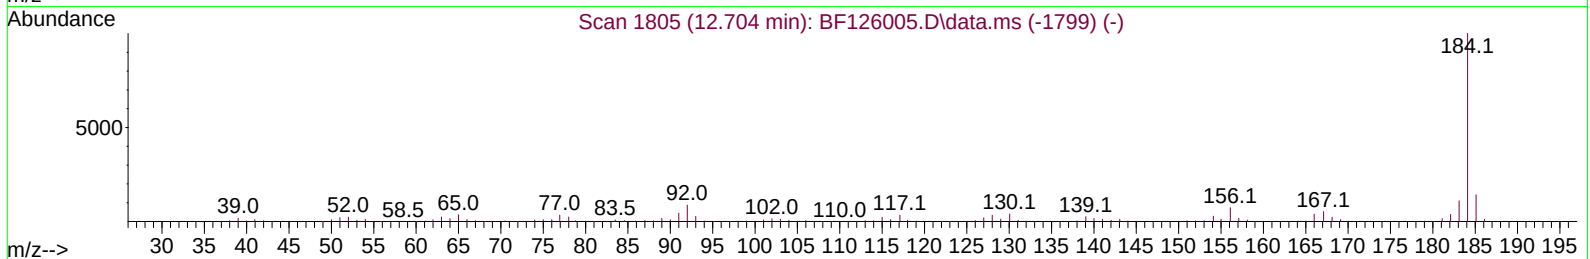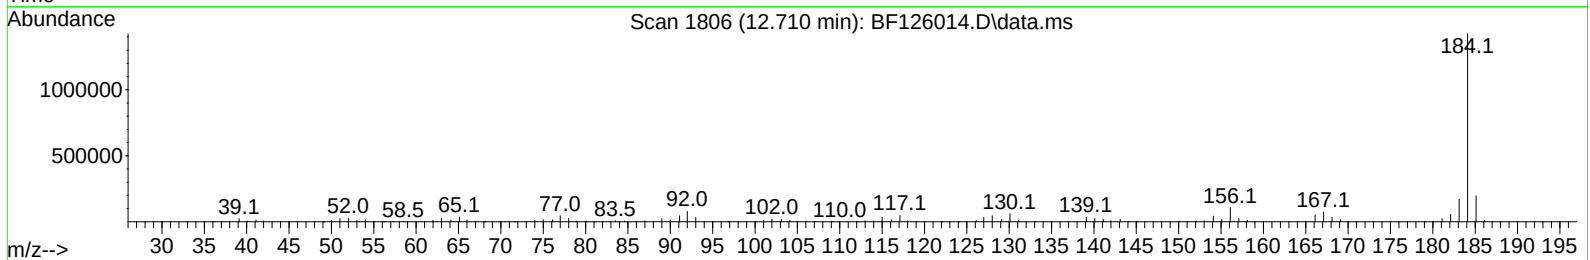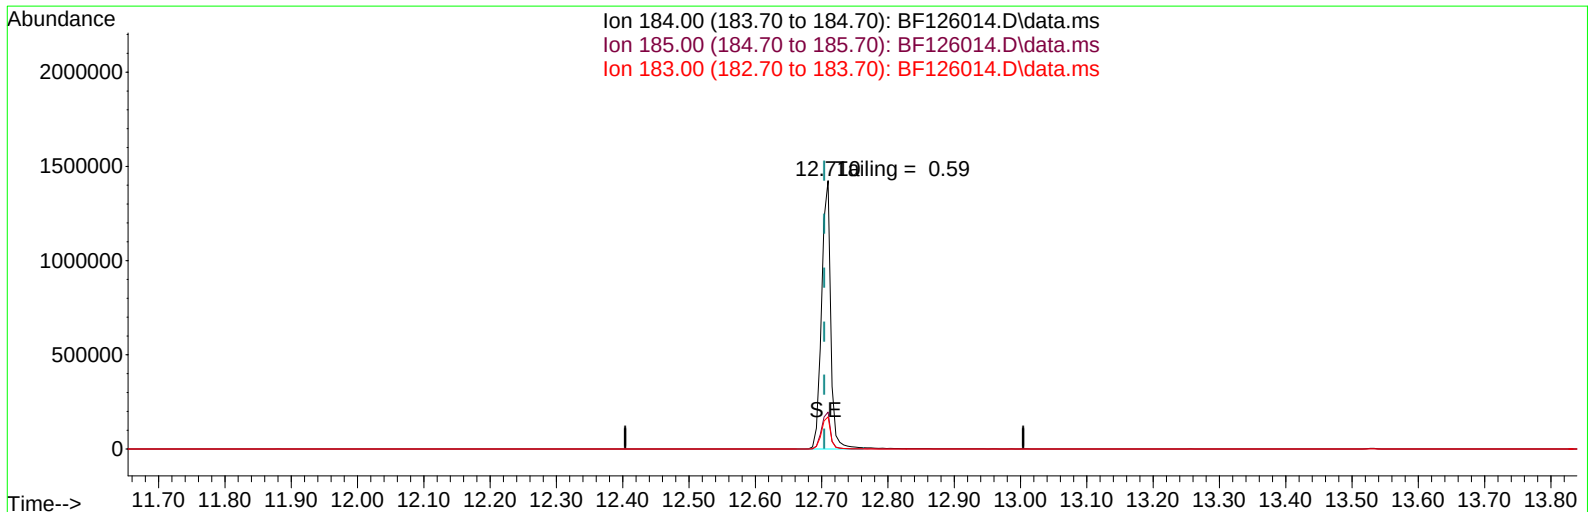

TIC: BF126014.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1362034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.81
183.00	10.10	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2021	BNA_F	BF126014.D
Compound Name	Response	Retention Time
DDT	463236	13.53
DDD	1975	13.23
DDE	360	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2335	465571	0.50