
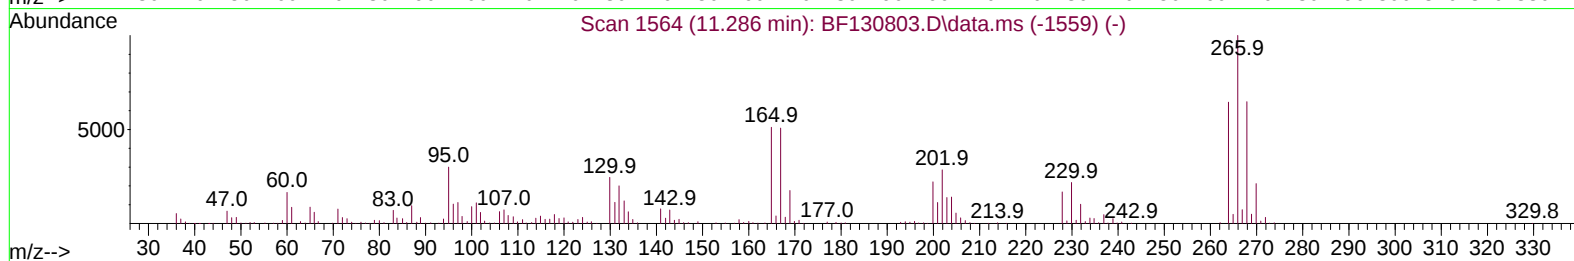
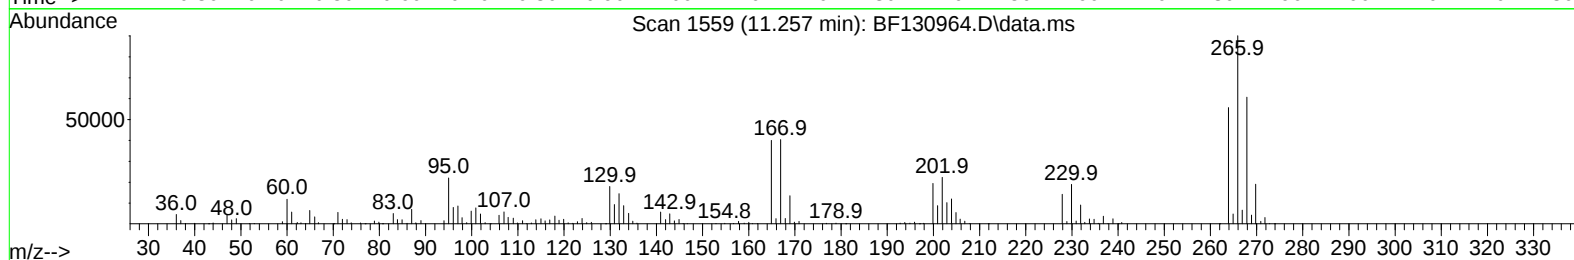


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\  
Data File : BF130964.D  
Acq On    : 03 Nov 2022  16:26  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 04 09:47:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

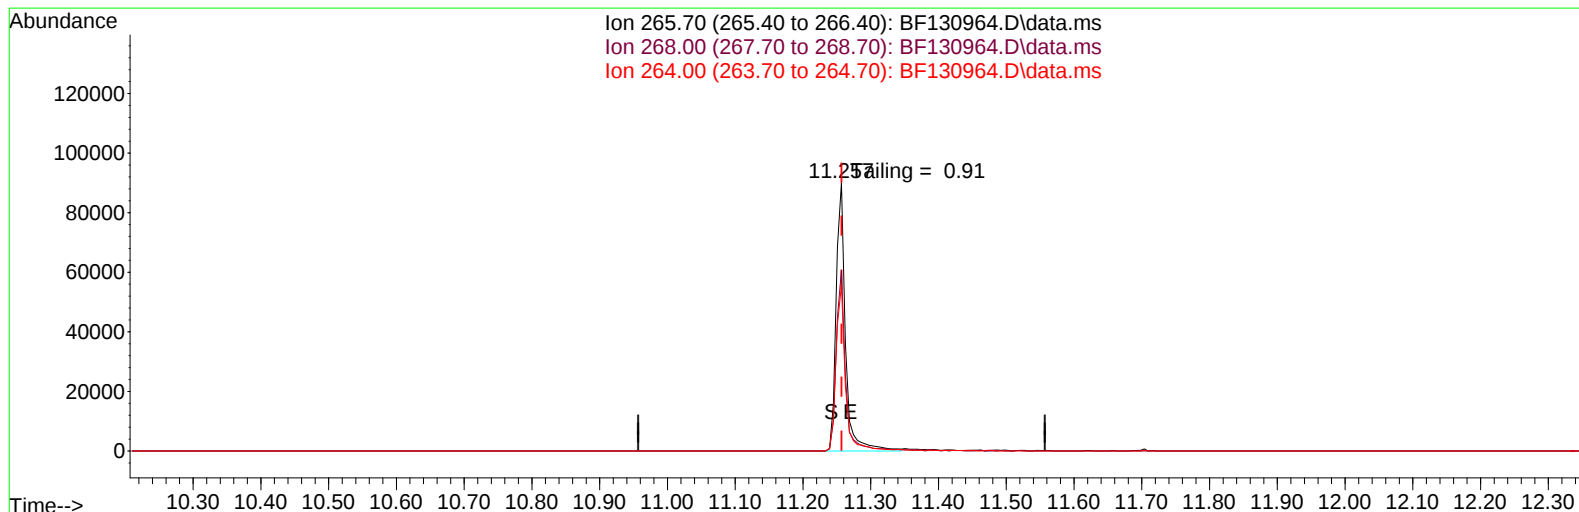

TIC: BF130964.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 27267.68 ng

response 86720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.39
264.00	64.50	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
 Data File : BF130964.D
 Acq On : 03 Nov 2022 16:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 09:47:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

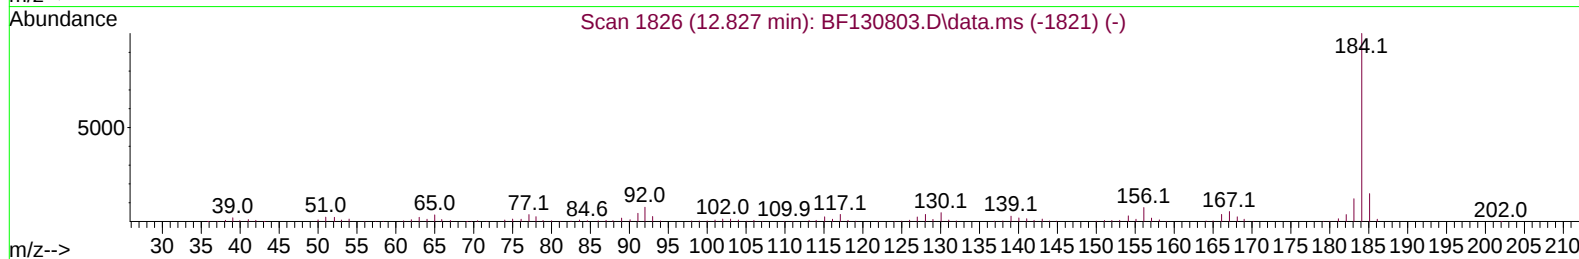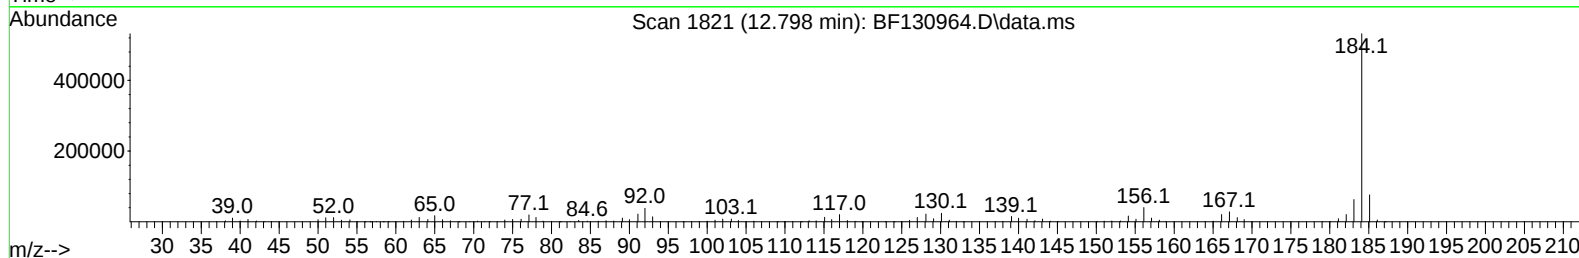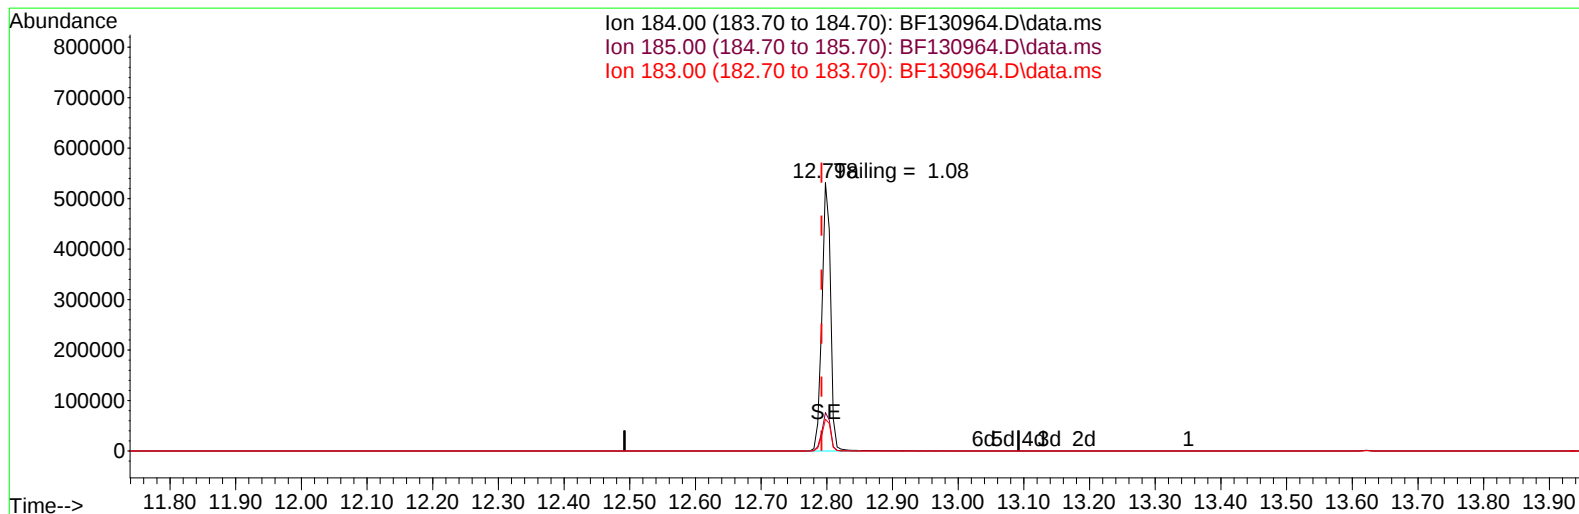

TIC: BF130964.D\data.ms

(77) Benzidine

12.798min (+ 0.006) 362934.67 ng m

response 484562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.31
183.00	12.10	11.89
0.00	0.00	0.00