
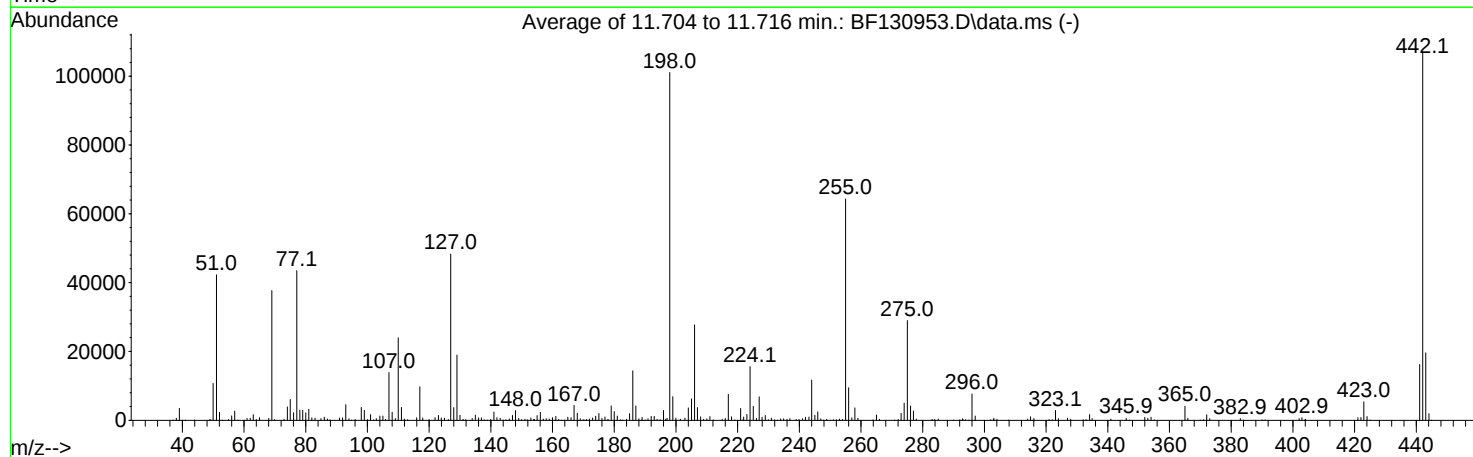


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
 Data File : BF130953.D
 Acq On : 03 Nov 2022 09:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:46:02 2022

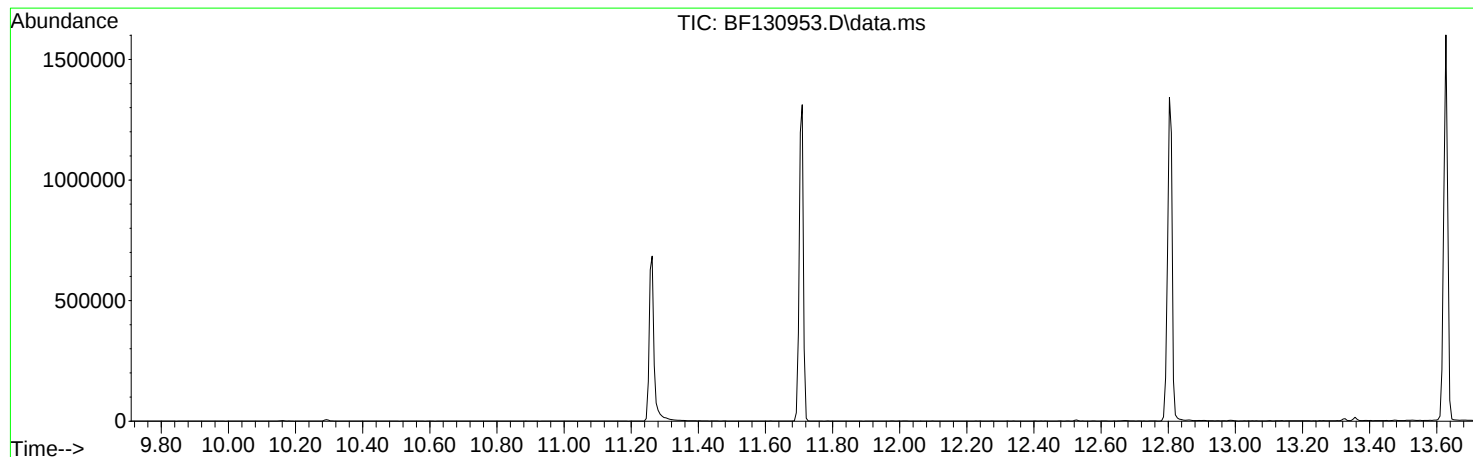




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	42286	PASS
68	69	0.00	2	1.6	595	PASS
69	198	0.00	100	37.3	37668	PASS
70	69	0.00	2	0.6	214	PASS
127	198	10	80	47.8	48282	PASS
197	198	0.00	2	0.6	565	PASS
198	198	100	100	100.0	101045	PASS
199	198	5	9	6.8	6881	PASS
275	198	10	60	28.7	28990	PASS
365	198	1	100	4.0	4082	PASS
441	198	0.01	100	16.0	16211	PASS
442	442	50	100	100.0	106899	PASS
443	442	15	24	18.3	19614	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
Data File : BF130953.D
Acq On : 03 Nov 2022 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 03 12:34:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 03:37:09 2022
Response via : Initial Calibration

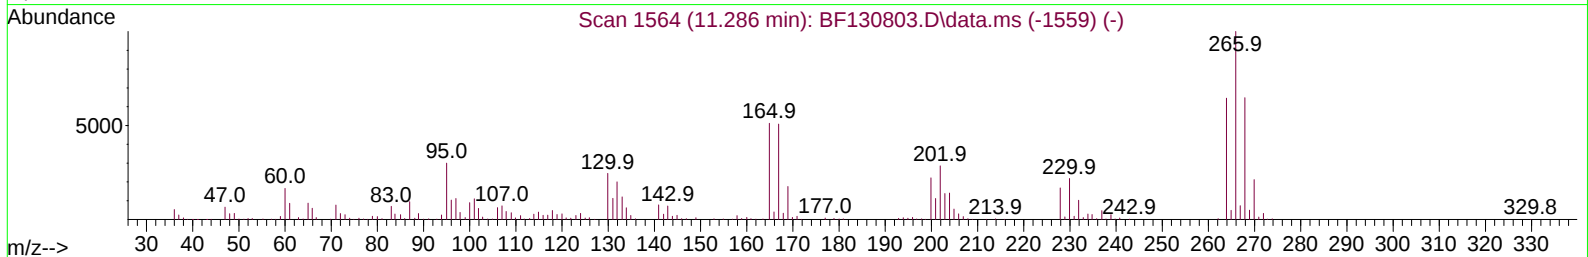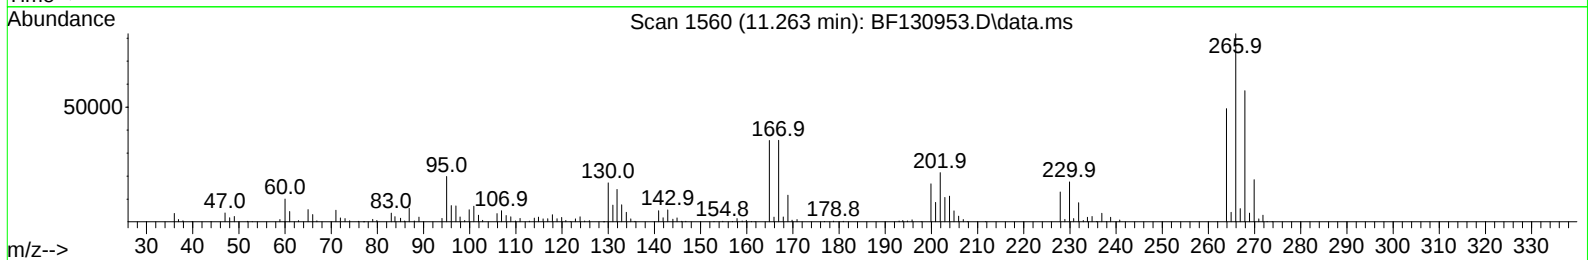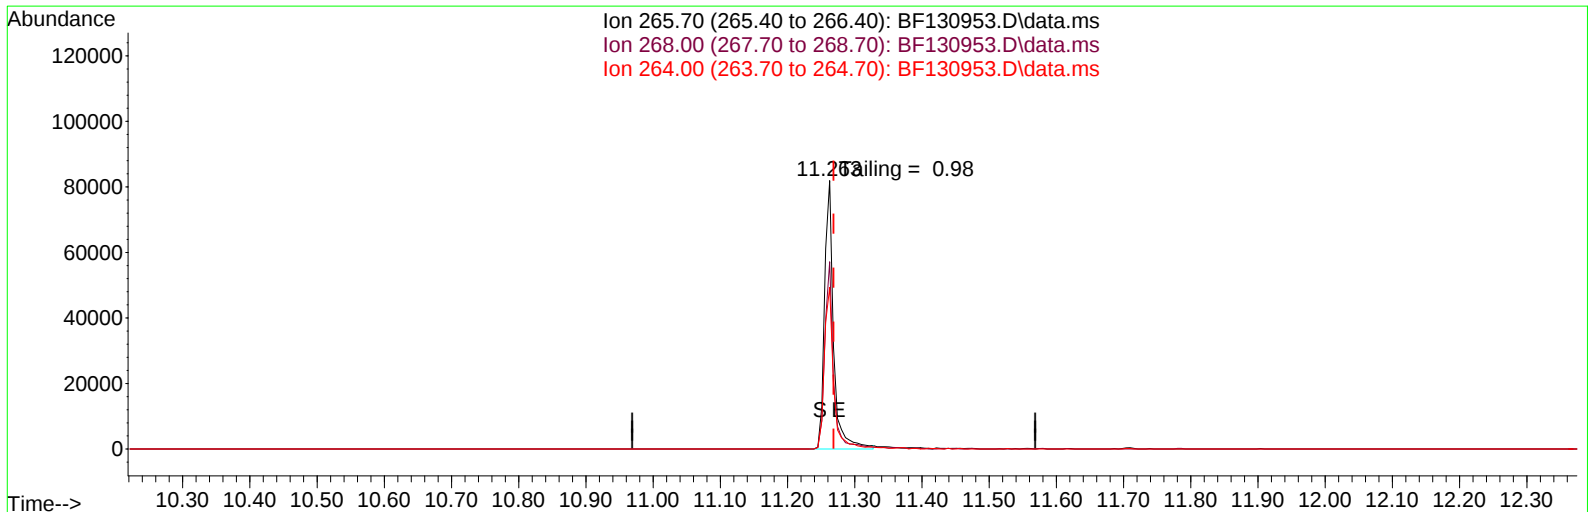

TIC: BF130953.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 22694.82 ng




response 78347

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	69.77
264.00	64.50	60.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
Data File : BF130953.D
Acq On : 03 Nov 2022 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 03 12:34:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 03:37:09 2022
Response via : Initial Calibration

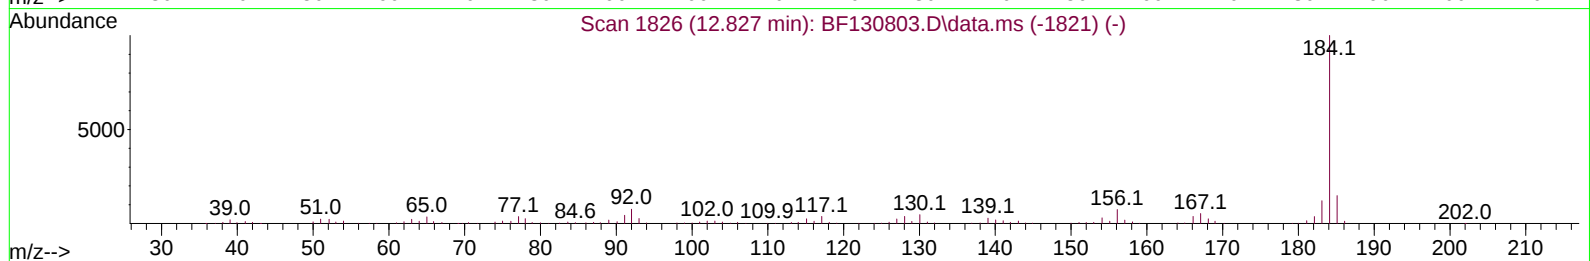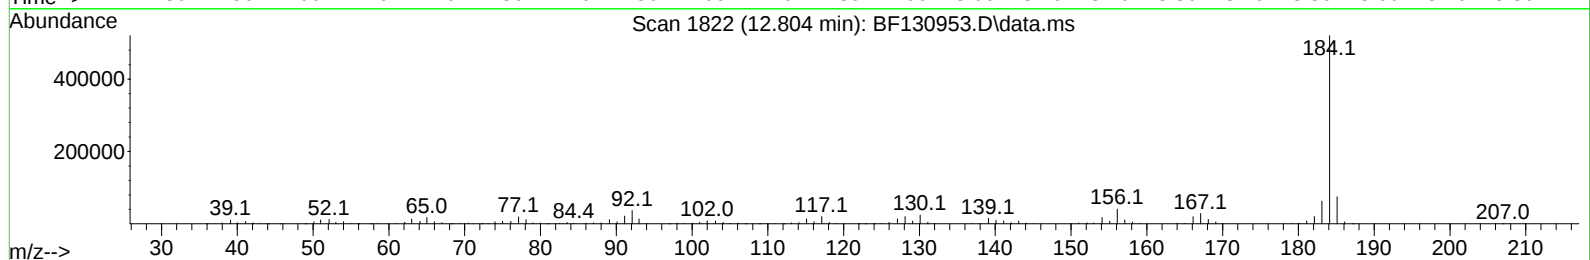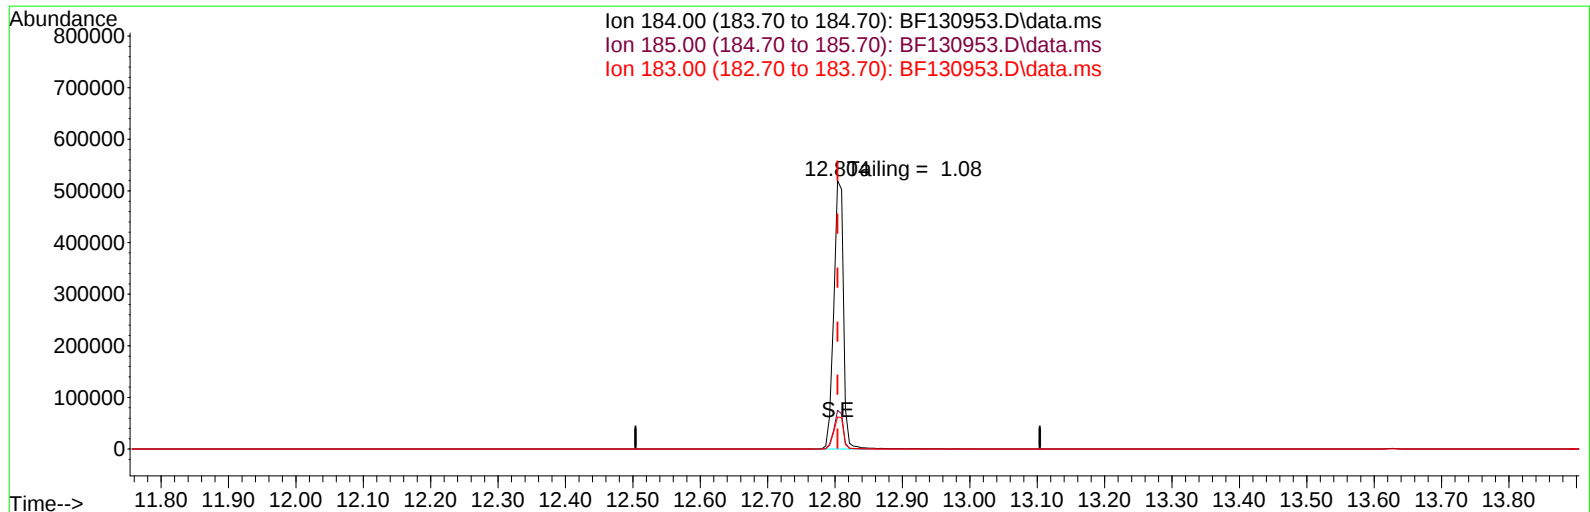

TIC: BF130953.D\data.ms

(77) Benzidine

12.804min (-0.000) 0.00 ng

response 518173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.43
183.00	12.10	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2022	BNA_F	<u>BF130953.D</u>
Compound Name	Response	Retention Time
DDT	250763	13.627
DDD	3941	13.357
DDE	501	12.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4442	255205	1.74

Instrument :
BNA_F
ClientSampleId :
DFTPP