


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
Data File : BF130964.D
Acq On : 03 Nov 2022 16:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 07 00:46:02 2022

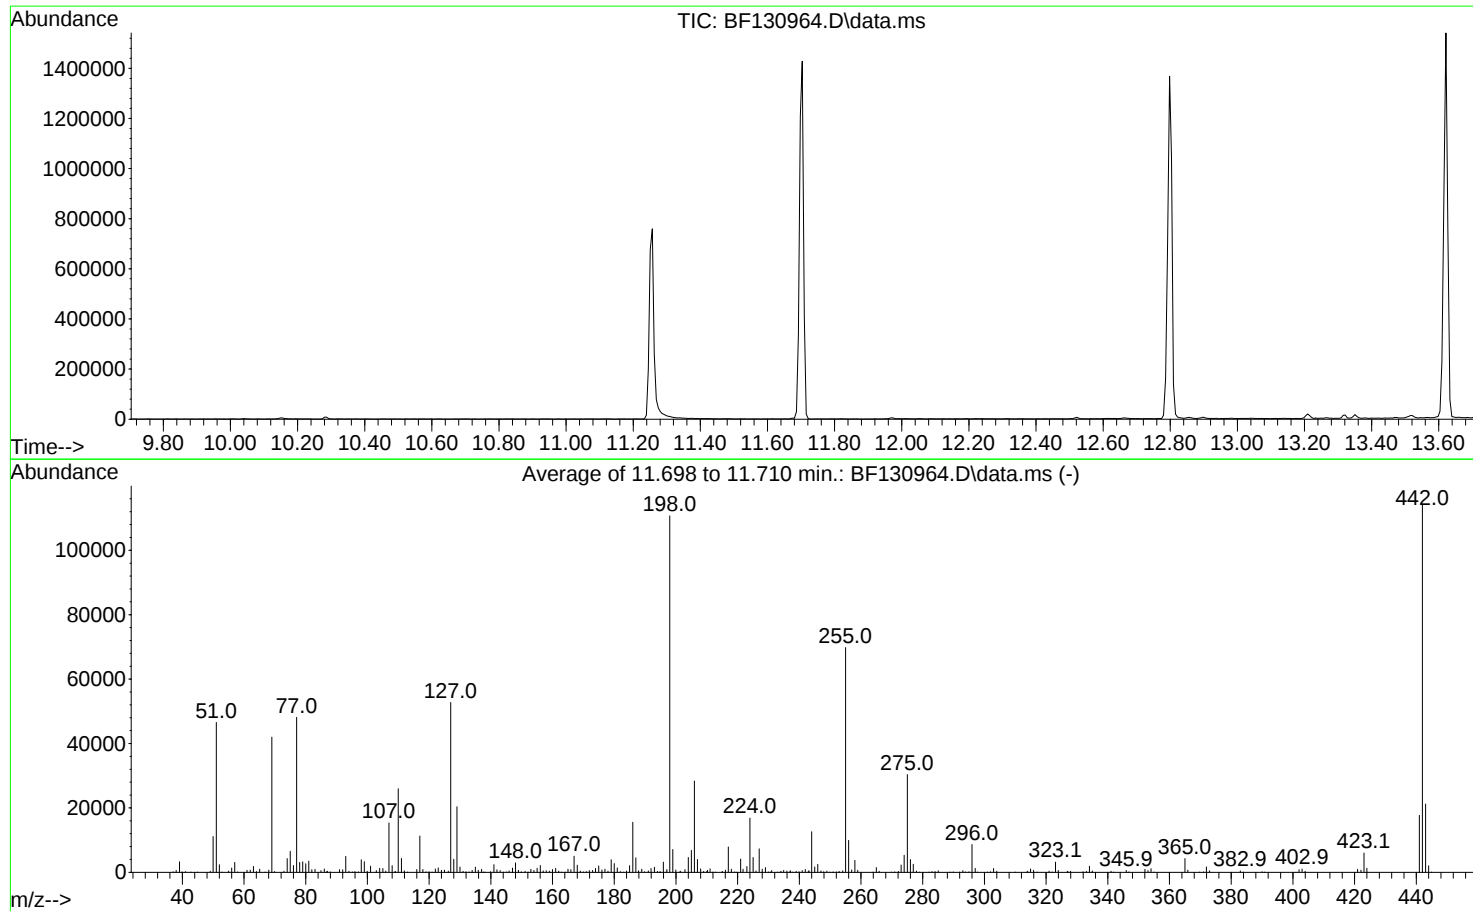




AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	46561	PASS
68	69	0.00	2	1.6	691	PASS
69	198	0.00	100	37.9	41989	PASS
70	69	0.00	2	0.6	248	PASS
127	198	10	80	47.7	52759	PASS
197	198	0.00	2	0.8	882	PASS
198	198	100	100	100.0	110688	PASS
199	198	5	9	6.4	7102	PASS
275	198	10	60	27.4	30361	PASS
365	198	1	100	3.8	4232	PASS
441	198	0.01	100	15.9	17647	PASS
442	442	50	100	100.0	114256	PASS
443	442	15	24	18.5	21191	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
 Data File : BF130964.D
 Acq On : 03 Nov 2022 16:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 04 09:47:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

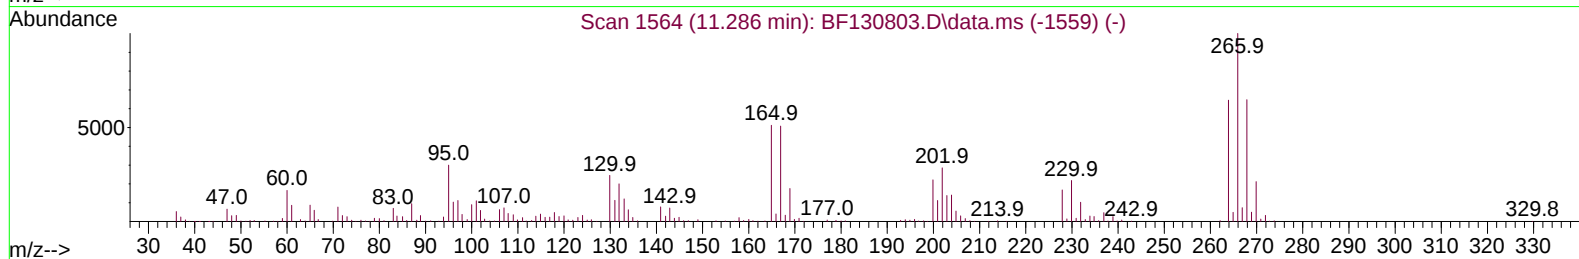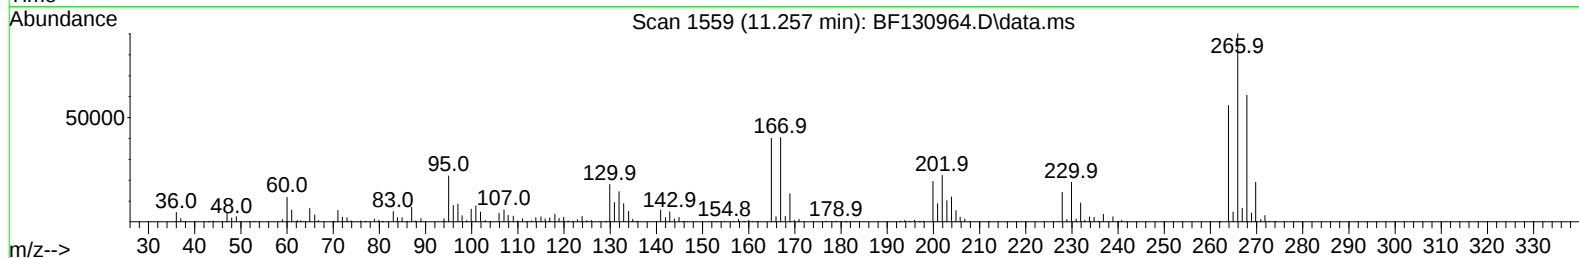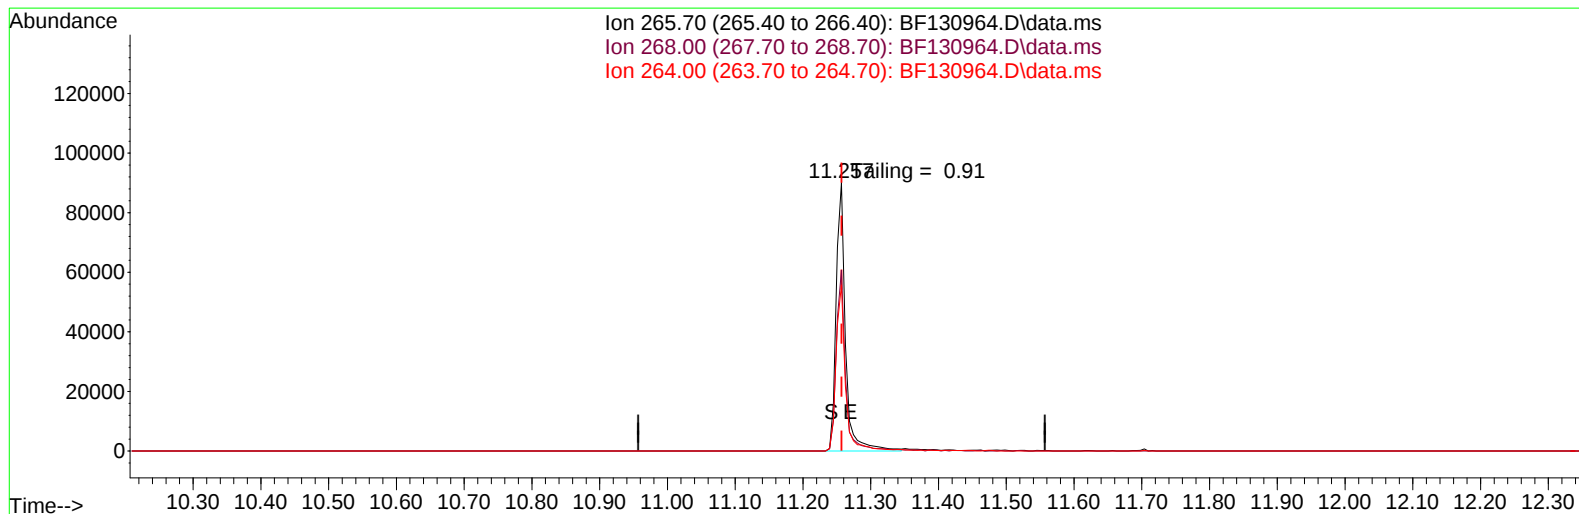

TIC: BF130964.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 27267.68 ng




response 86720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.39
264.00	64.50	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110322\
 Data File : BF130964.D
 Acq On : 03 Nov 2022 16:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 04 09:47:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

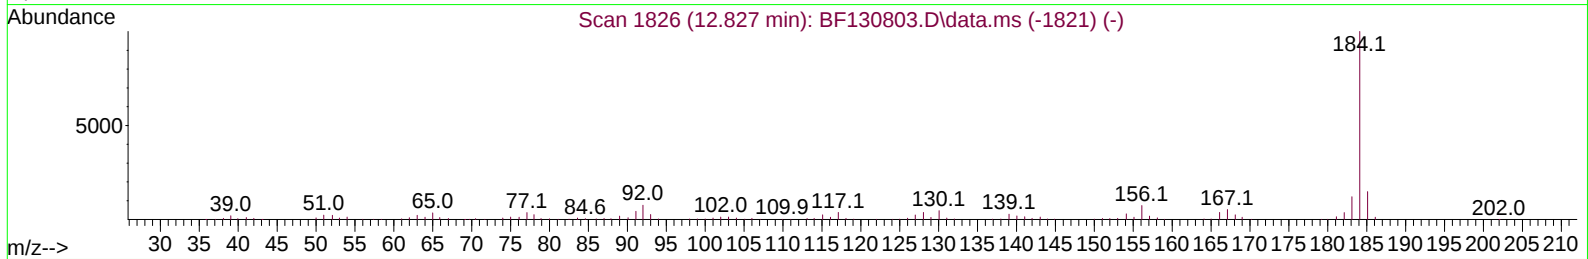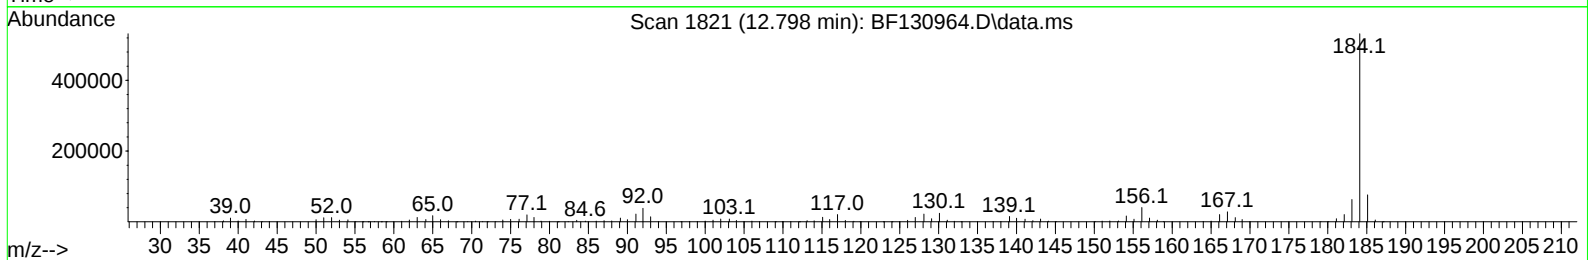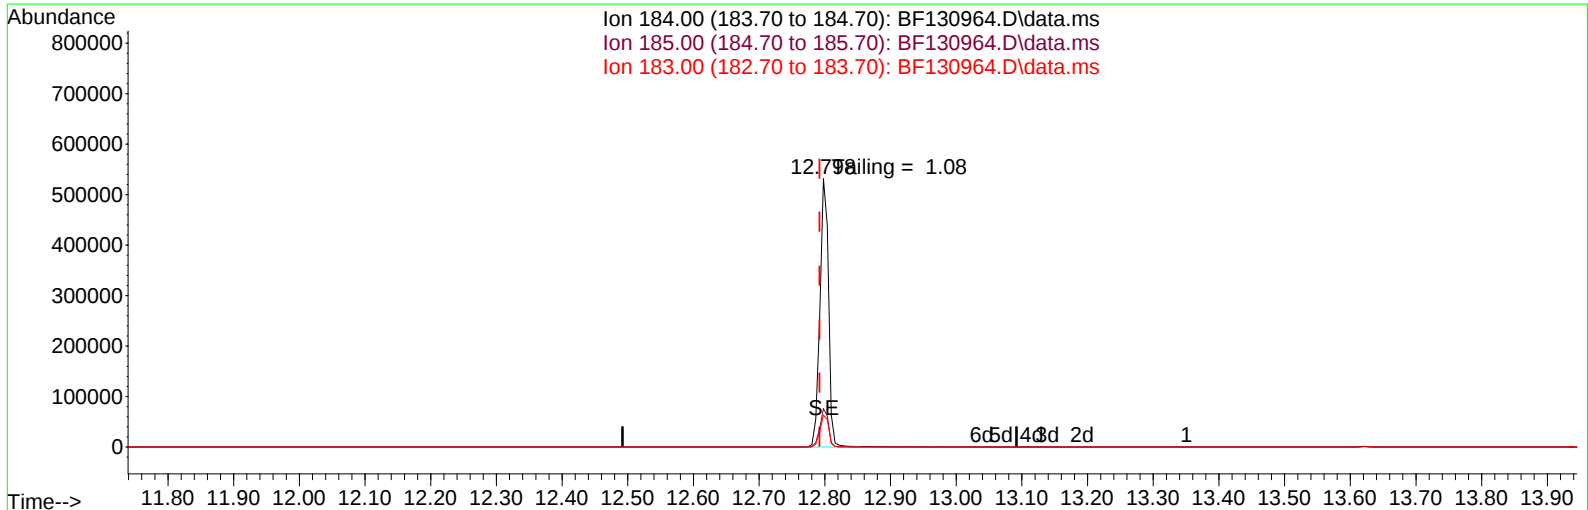

TIC: BF130964.D\data.ms

(77) Benzidine

12.798min (+ 0.006) 362934.67 ng m

response 484562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.31
183.00	12.10	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2022	BNA_F	<u>BF130964.D</u>
Compound Name	Response	Retention Time
DDT	238092	13.621
DDD	5244	13.321
DDE	245	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5489	243581	2.25

Instrument :
BNA_F
ClientSampleId :
DFTPP