
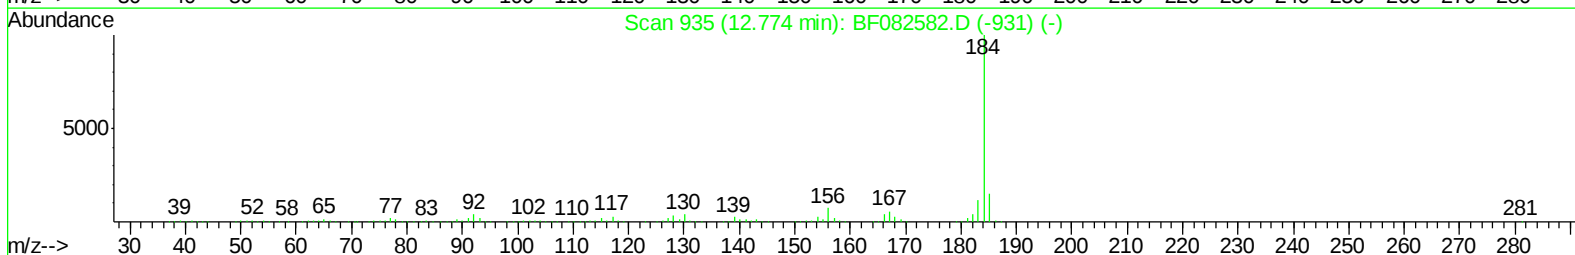
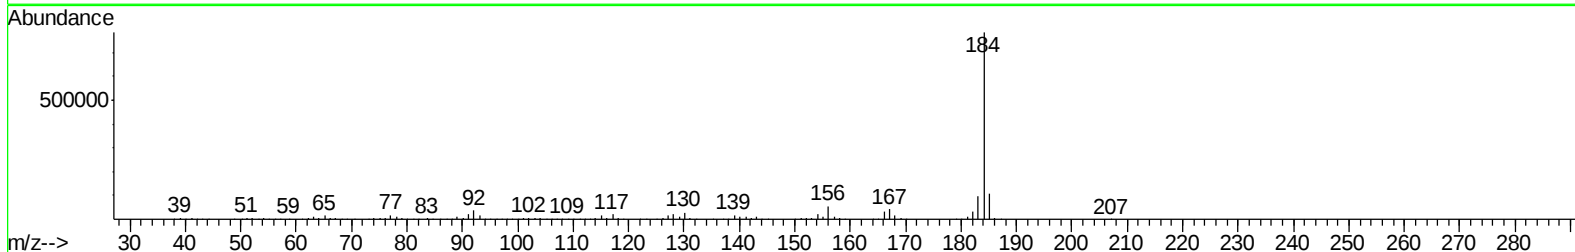


Data Path : Z:\HPCHEM1\BNA F\Data\BF110415\
Data File : BF082676.D
Acq On : 4 Nov 2015 1:14
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 08:19:54 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

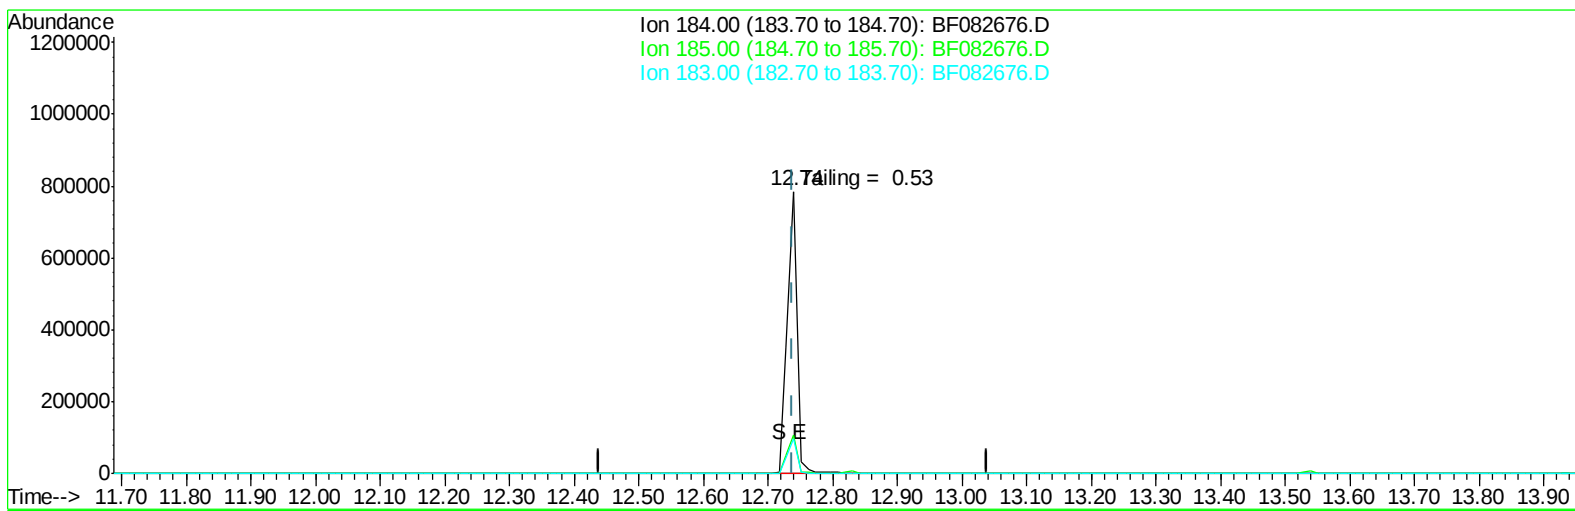

TIC: BF082676.D

(76) Benzidine




12.739min (+0.000) 39691.64ng

response 827006

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.71
183.00	12.00	12.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF110415\
Data File : BF082676.D
Acq On : 4 Nov 2015 1:14
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 08:19:54 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

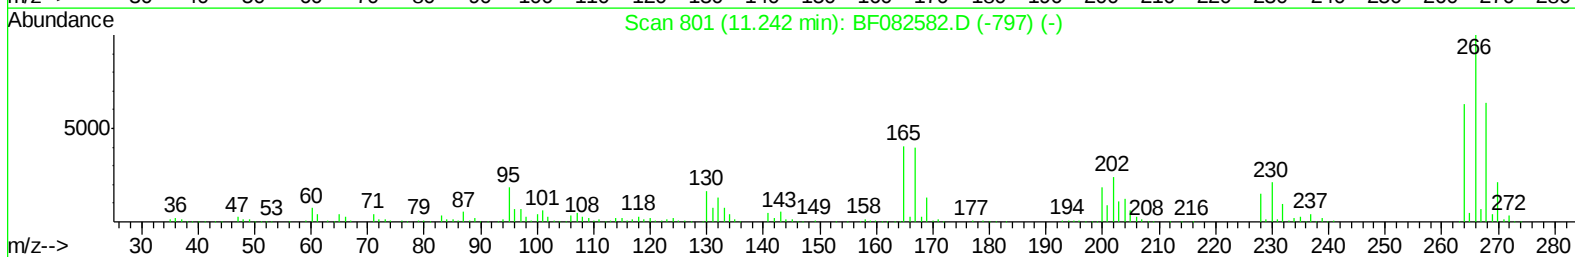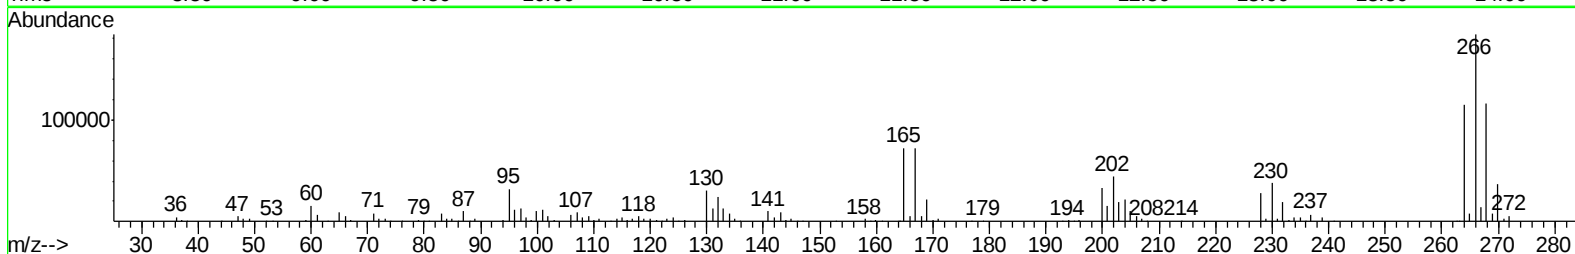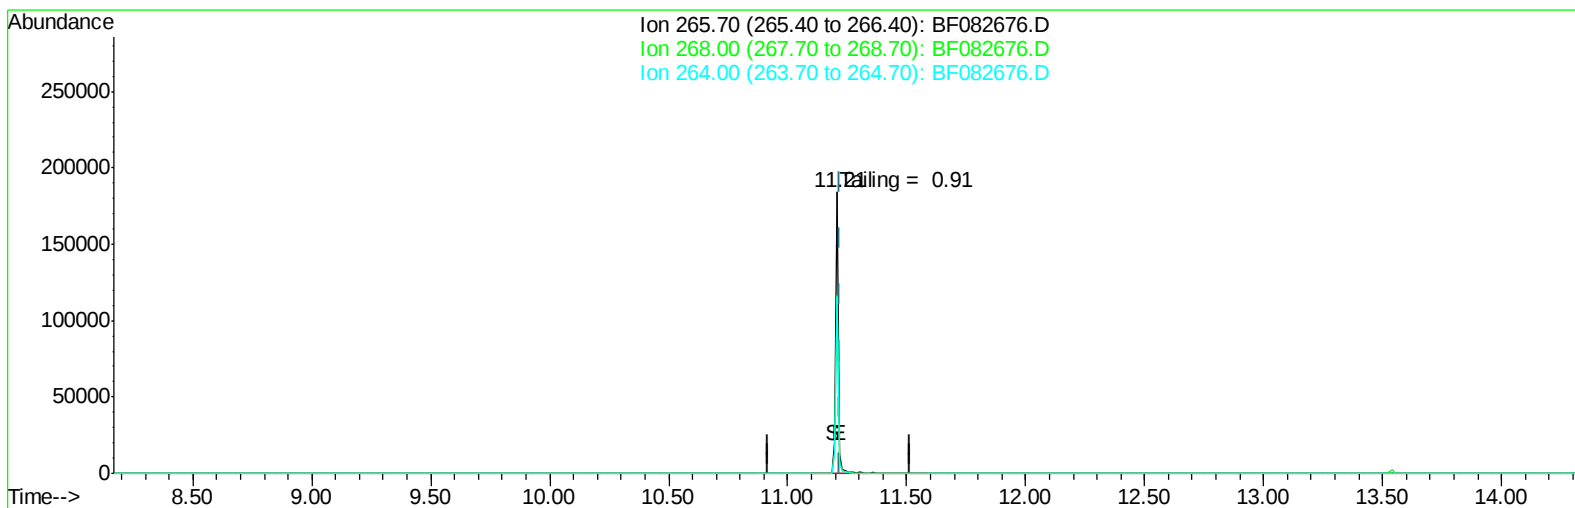

TIC: BF082676.D

(69) Pentachlorophenol (C)

11.208min (-0.011) 0.00ng

response 154013

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	63.26
264.00	63.20	62.76
0.00	0.00	0.00