


Data Path : Z:\HPCHEM1\BNA F\Data\BF110415\
 Data File : BF082676.D
 Acq On : 4 Nov 2015 1:14
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 03 12:27:47 2015

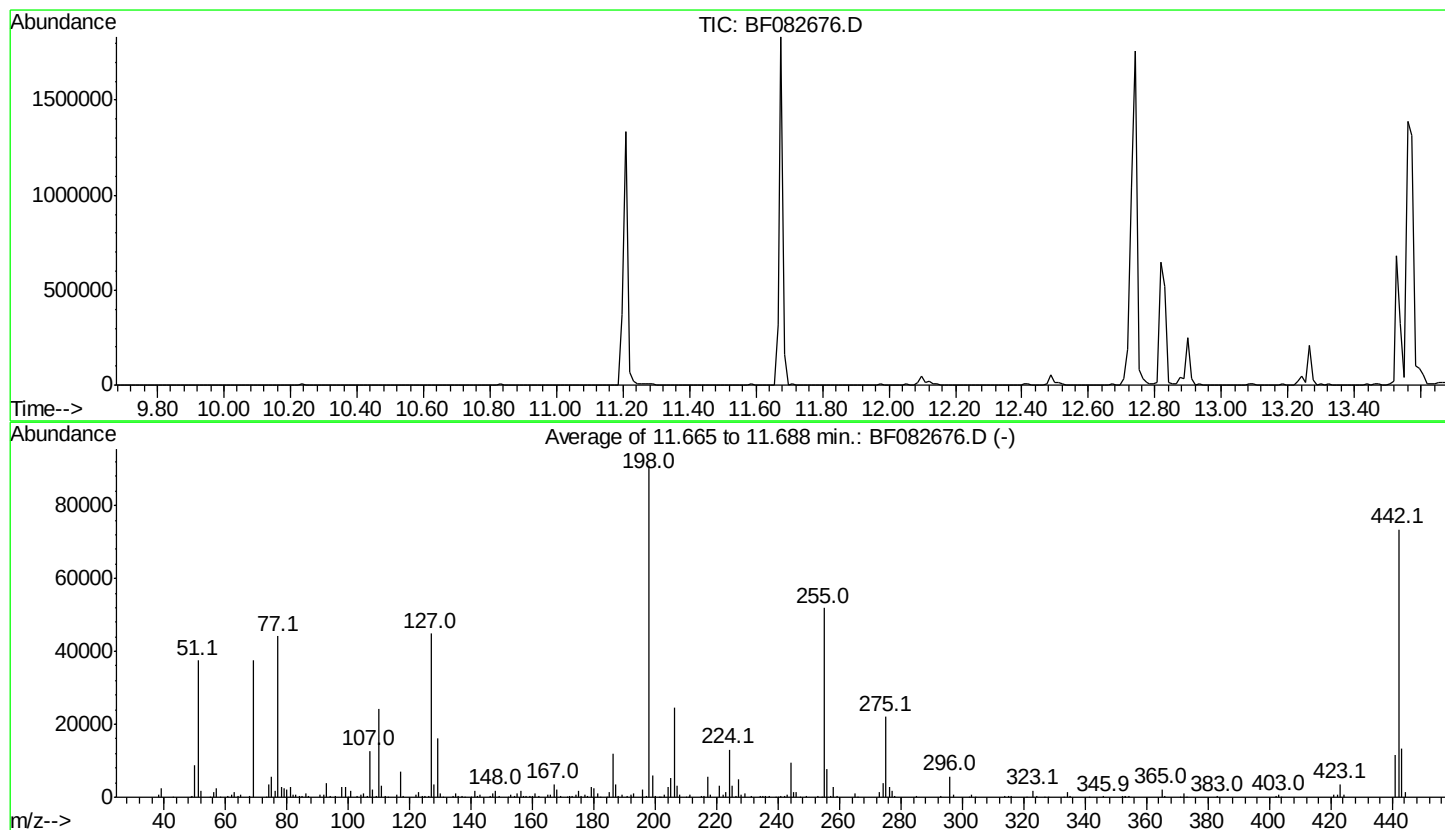

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	37476	PASS
68	69	0.00	2	1.4	535	PASS
69	198	0.00	100	41.1	37412	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	44807	PASS
197	198	0.00	2	0.6	518	PASS
198	198	100	100	100.0	90935	PASS
199	198	5	9	6.6	5977	PASS
275	198	10	60	24.3	22063	PASS
365	198	1	100	2.5	2265	PASS
441	442	0.01	24	15.6	11494	PASS
442	198	50	100	80.9	73546	PASS
443	442	15	24	18.2	13372	PASS