
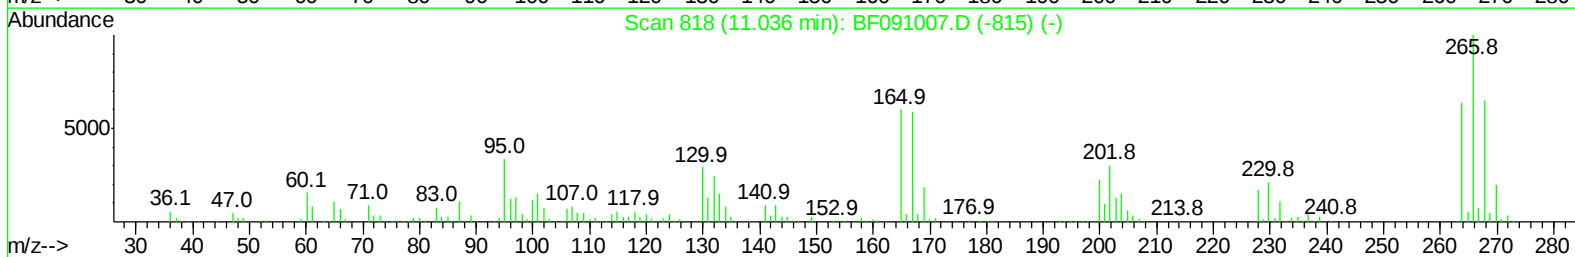
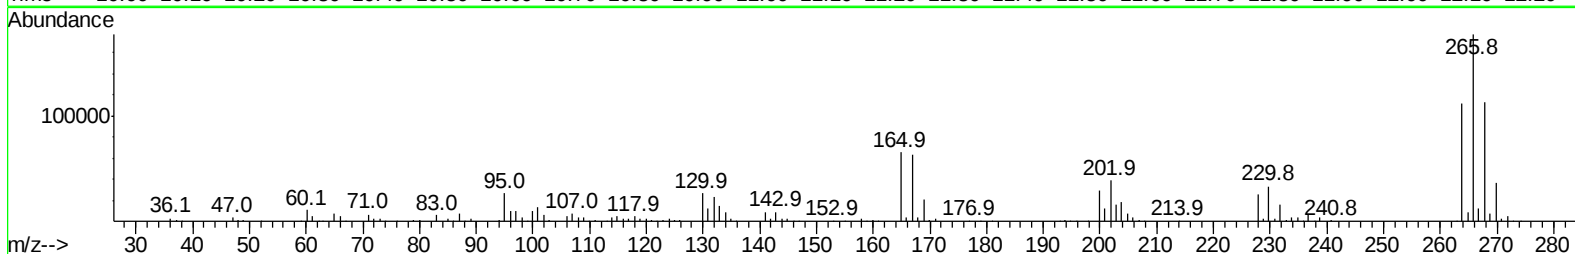


Data Path : Z:\HPCHEM1\BNA F\Data\BF110416\
Data File : BF091012.D
Acq On : 4 Nov 2016 8:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 18:08:03 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 11:03:12 2016
Response via : Initial Calibration

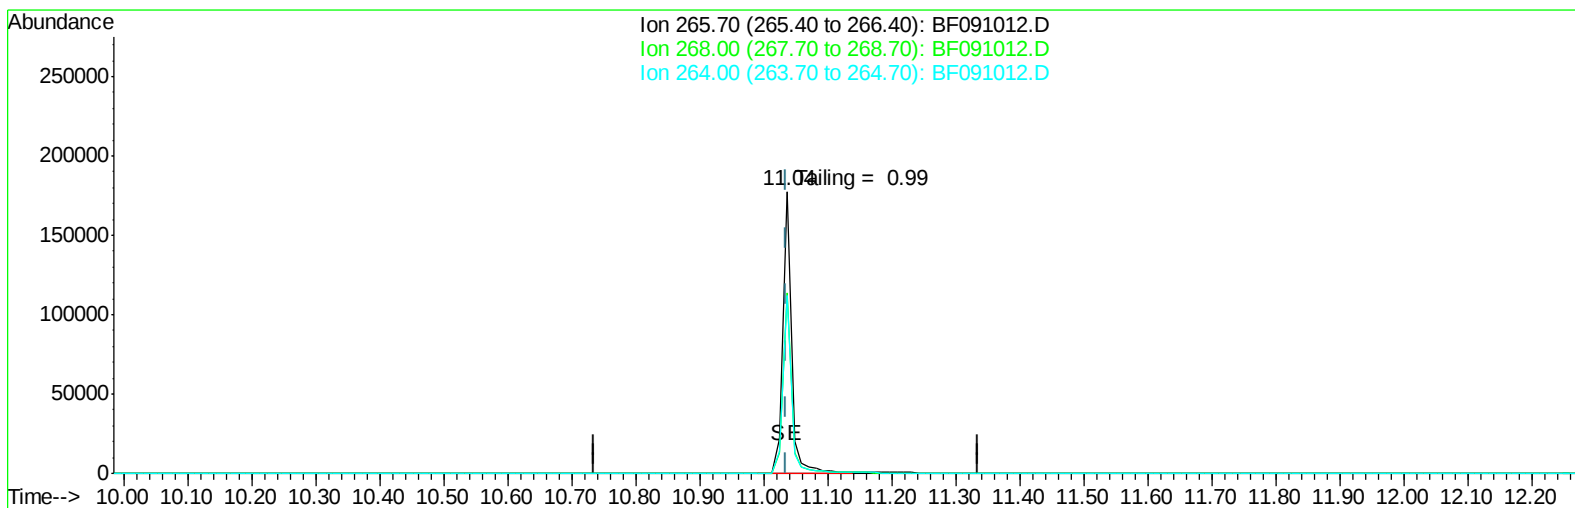

TIC: BF091012.D

(69) Pentachlorophenol (C)




11.036min (+0.000) 61222.81ng

response 167359

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.05
264.00	63.90	63.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF110416\
Data File : BF091012.D
Acq On : 4 Nov 2016 8:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 18:08:03 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 11:03:12 2016
Response via : Initial Calibration

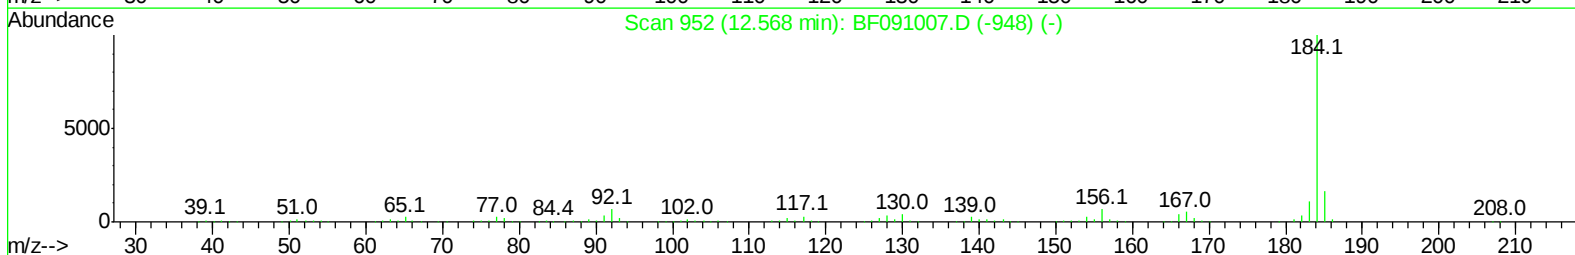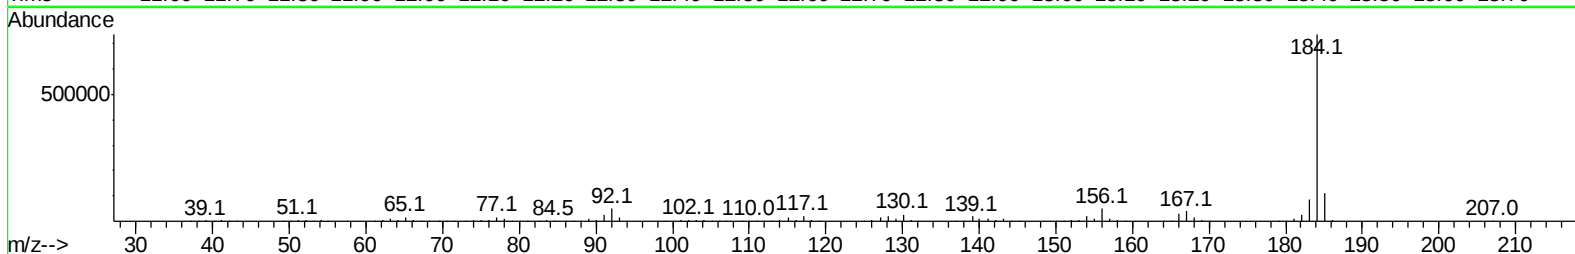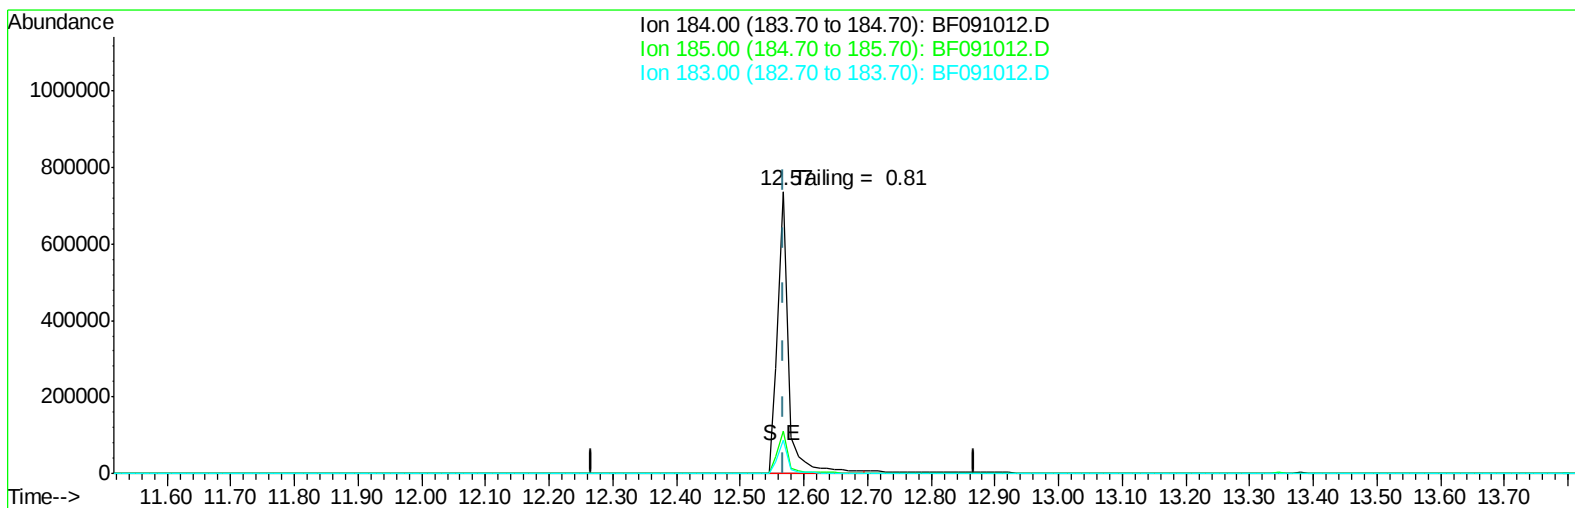

TIC: BF091012.D

(76) Benzidine

12.568min (+0.000) 34727.83ng

response 897646

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.80
183.00	10.90	11.75
0.00	0.00	0.00