
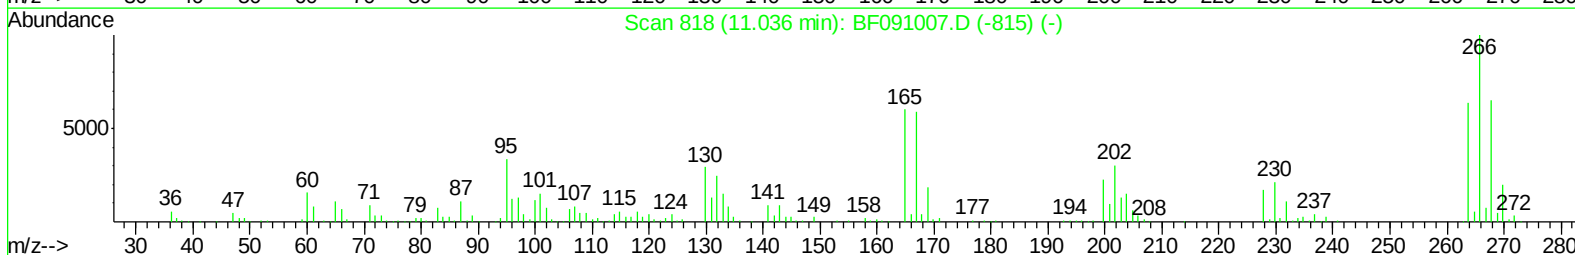
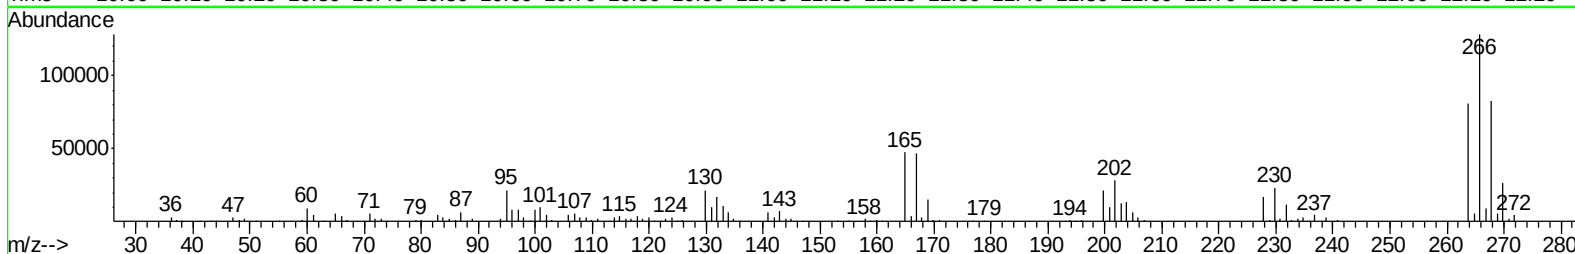


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110416\
Data File : BF091026.D
Acq On : 4 Nov 2016 17:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 05:04:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 11:03:12 2016
Response via : Initial Calibration

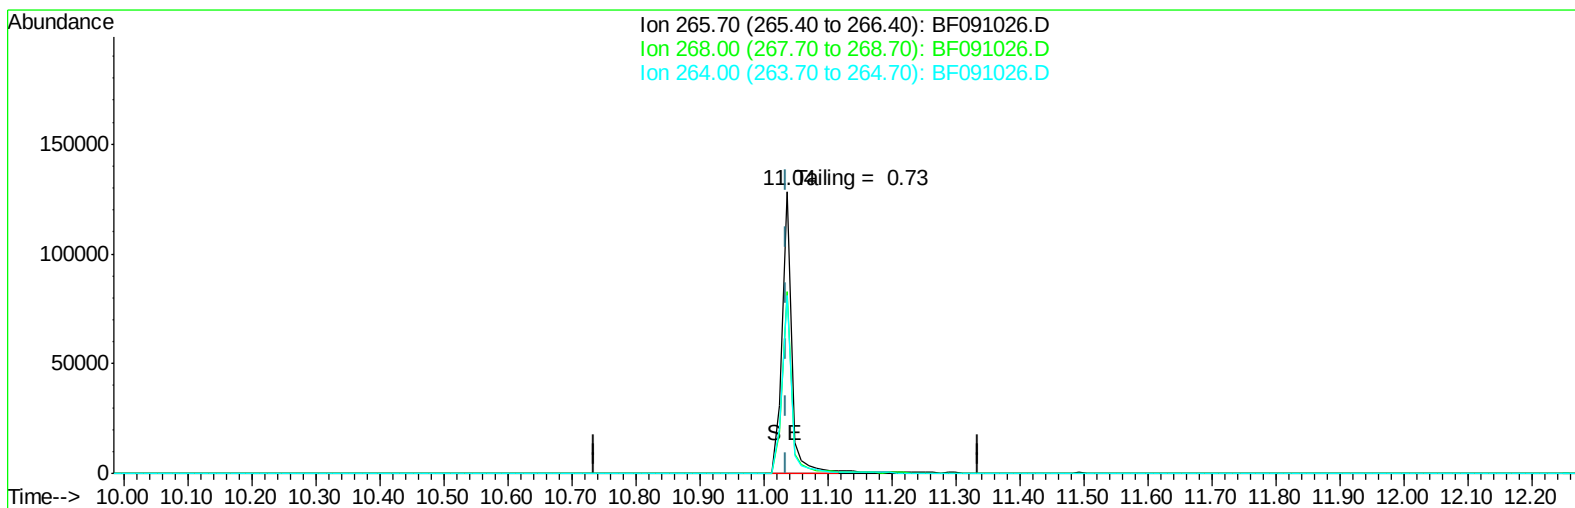

TIC: BF091026.D

(69) Pentachlorophenol (C)




11.036min (+0.000) 0.00ng

response 135255

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.55
264.00	63.90	63.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110416\
Data File : BF091026.D
Acq On : 4 Nov 2016 17:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 05:04:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 11:03:12 2016
Response via : Initial Calibration

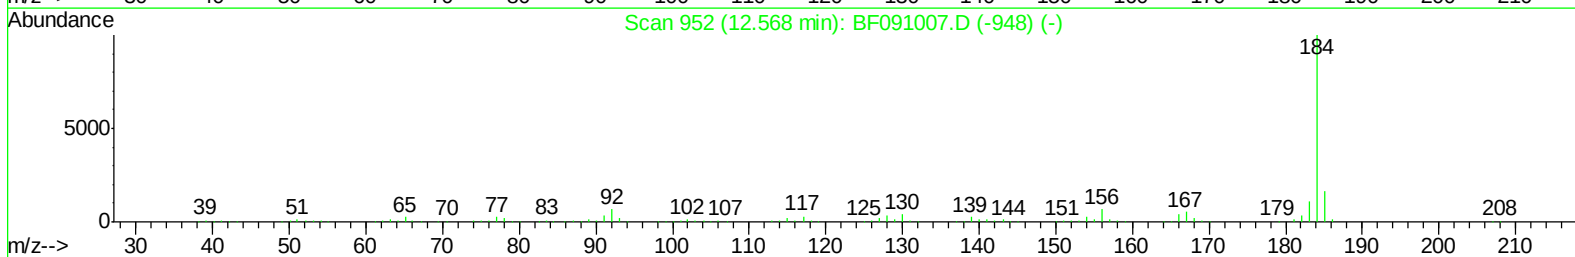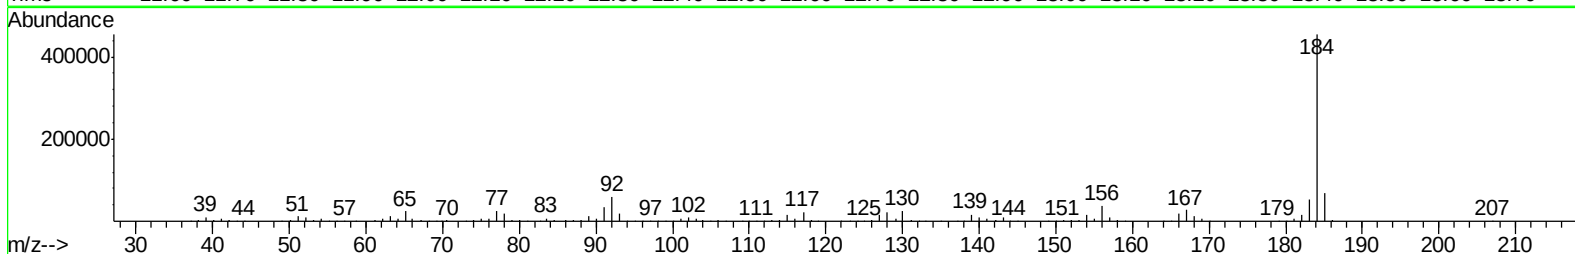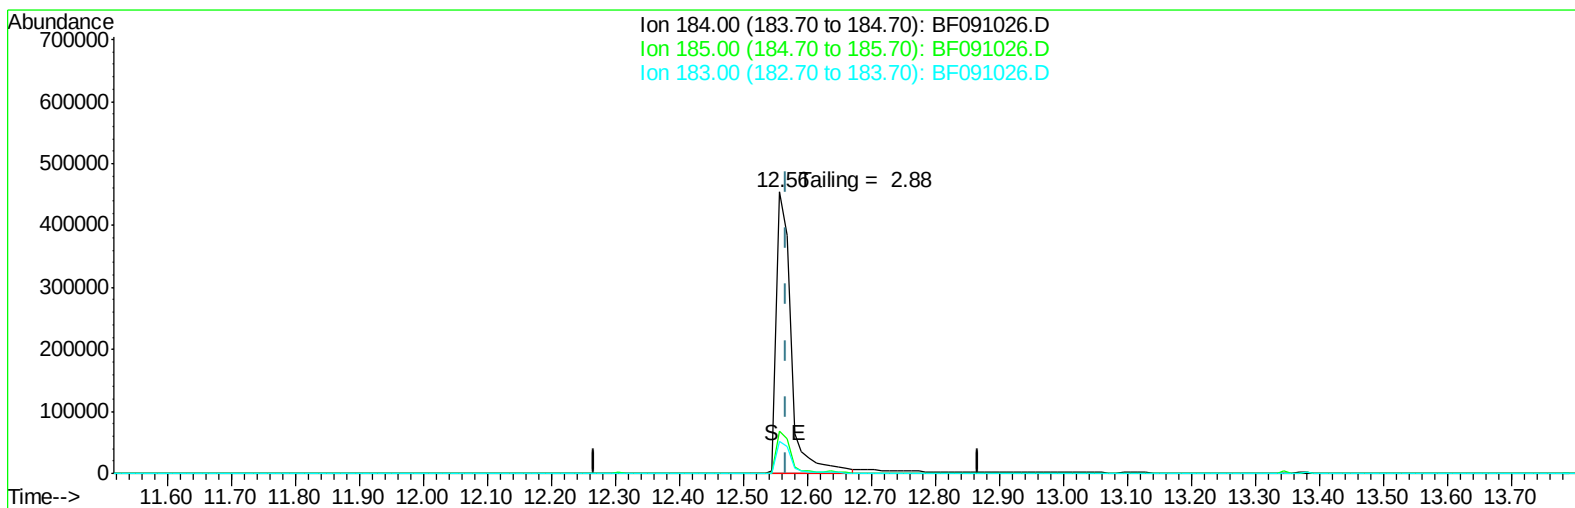

TIC: BF091026.D

(76) Benzidine

12.557min (-0.011) 123575.22ng

response 742639

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.15
183.00	10.90	11.60
0.00	0.00	0.00