


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110416\
 Data File : BF091012.D
 Acq On : 4 Nov 2016 8:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 11:03:12 2016

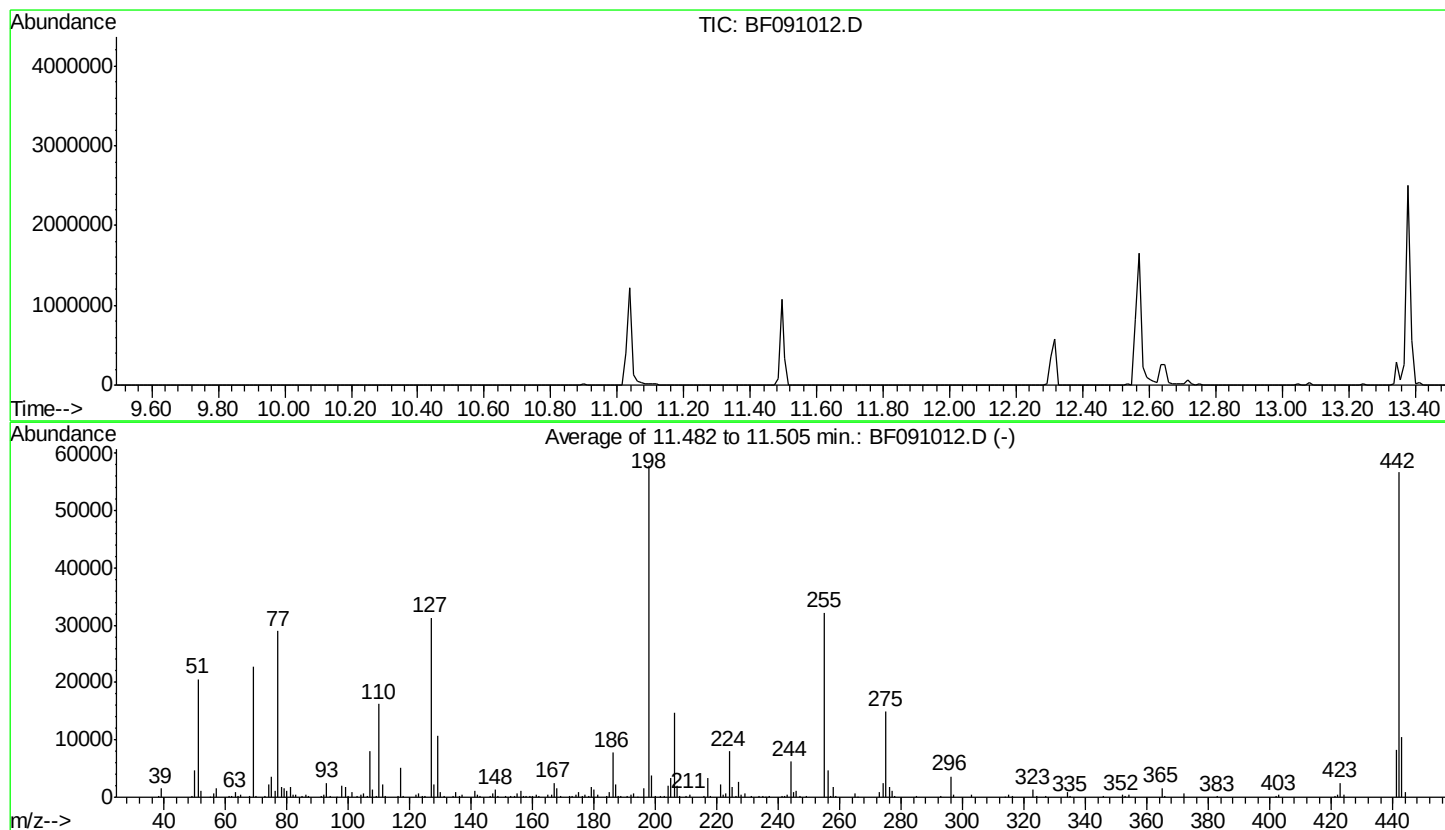

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	20589	PASS
68	69	0.00	2	1.2	274	PASS
69	198	0.00	100	39.5	22825	PASS
70	69	0.00	2	0.6	135	PASS
127	198	10	80	54.1	31263	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57815	PASS
199	198	5	9	6.7	3872	PASS
275	198	10	60	25.7	14874	PASS
365	198	1	100	2.9	1655	PASS
441	442	0.01	24	14.7	8371	PASS
442	198	50	100	98.2	56770	PASS
443	442	15	24	18.5	10481	PASS