


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110416\
 Data File : BF091026.D
 Acq On : 4 Nov 2016 17:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 11:03:12 2016

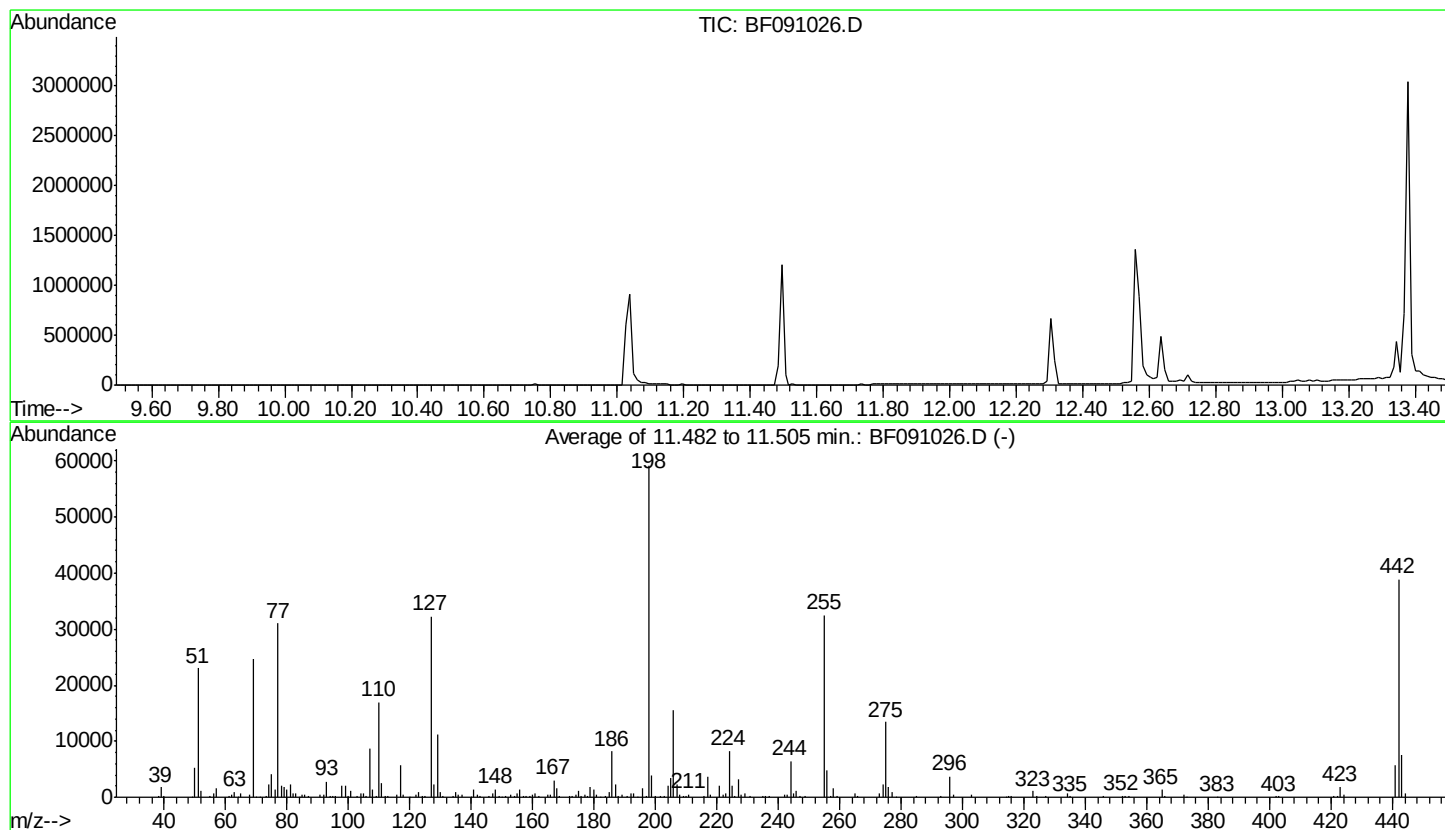

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	23068	PASS
68	69	0.00	2	1.7	429	PASS
69	198	0.00	100	41.7	24694	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	54.4	32220	PASS
197	198	0.00	2	0.3	176	PASS
198	198	100	100	100.0	59192	PASS
199	198	5	9	6.6	3894	PASS
275	198	10	60	22.7	13452	PASS
365	198	1	100	2.3	1332	PASS
441	442	0.01	24	15.0	5824	PASS
442	198	50	100	65.7	38907	PASS
443	442	15	24	19.4	7532	PASS