
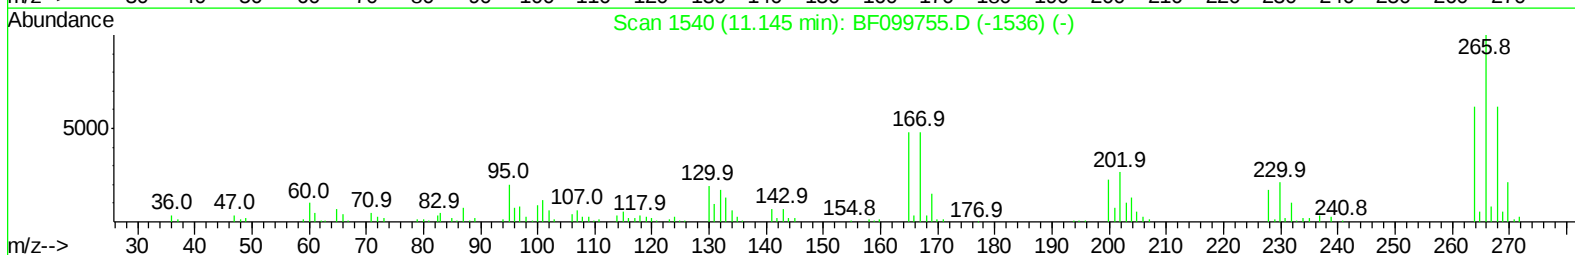
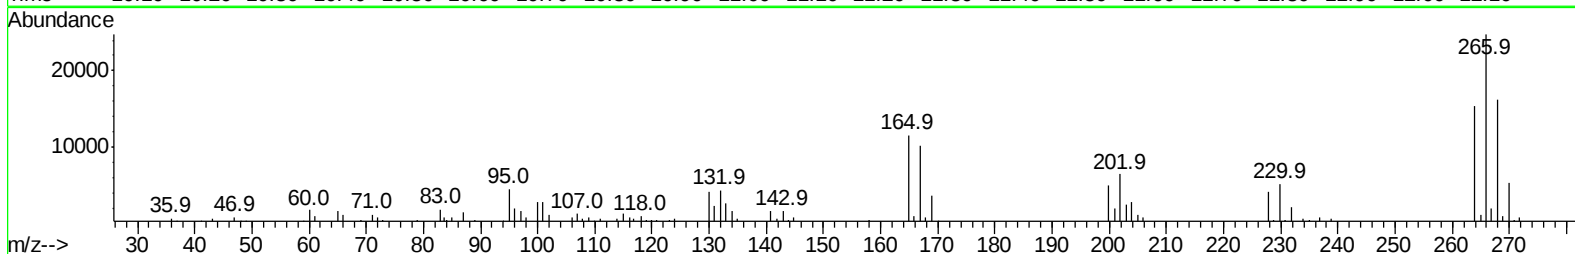


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100170.D
 Acq On : 4 Nov 2017 10:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 06 04:49:57 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 03 15:46:10 2017
 Response via : Initial Calibration

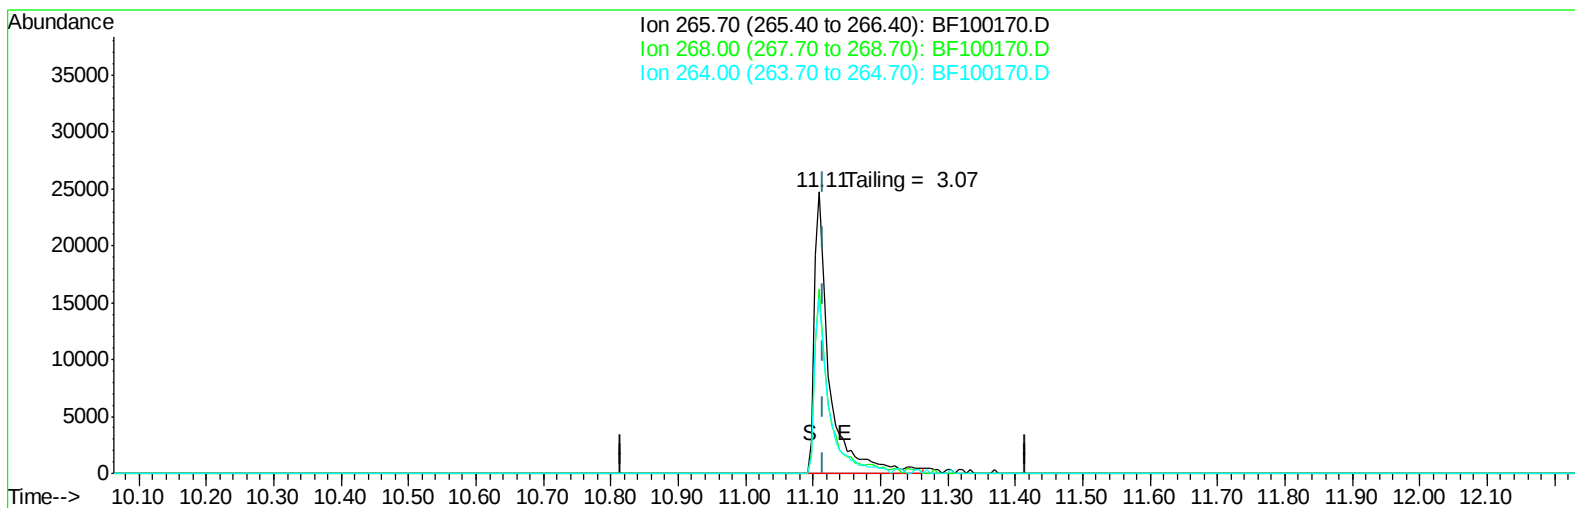

TIC: BF100170.D

(69) Pentachlorophenol (C)

11.110min (-0.006) 68388.22ng

response 36509

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.62
264.00	61.90	62.40
0.00	0.00	0.00

