
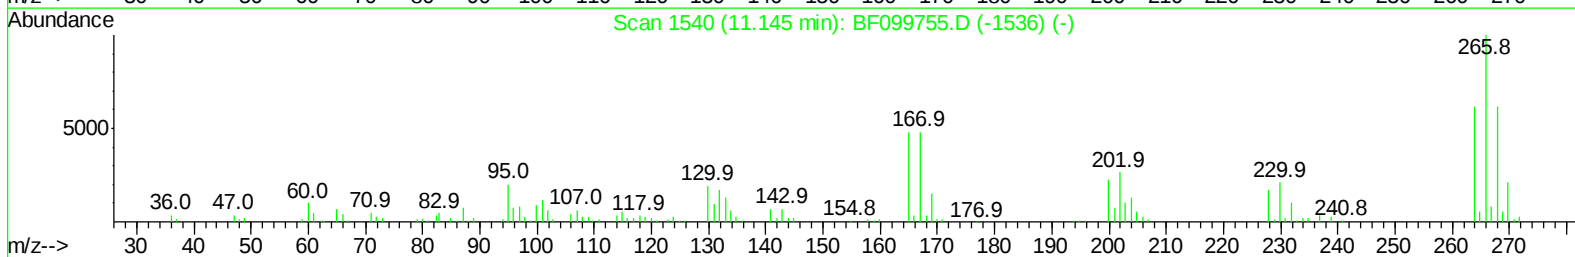
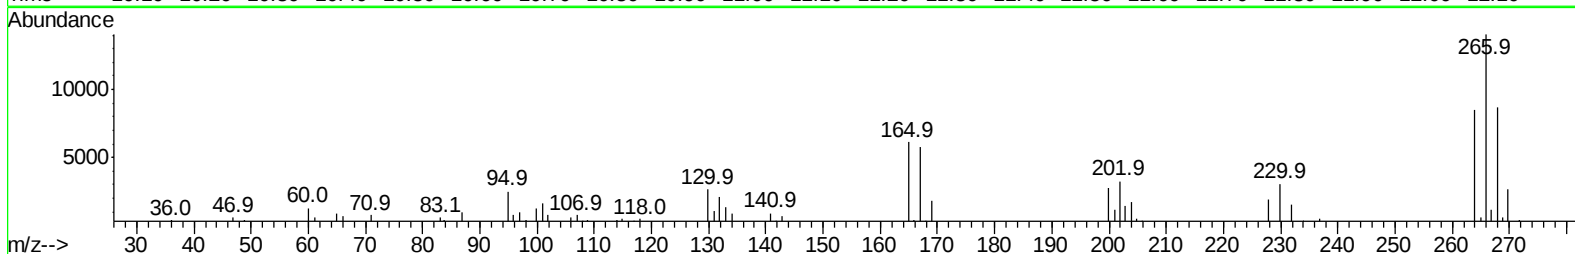


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100195.D
Acq On : 4 Nov 2017 22:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 04:53:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:46:10 2017
Response via : Initial Calibration

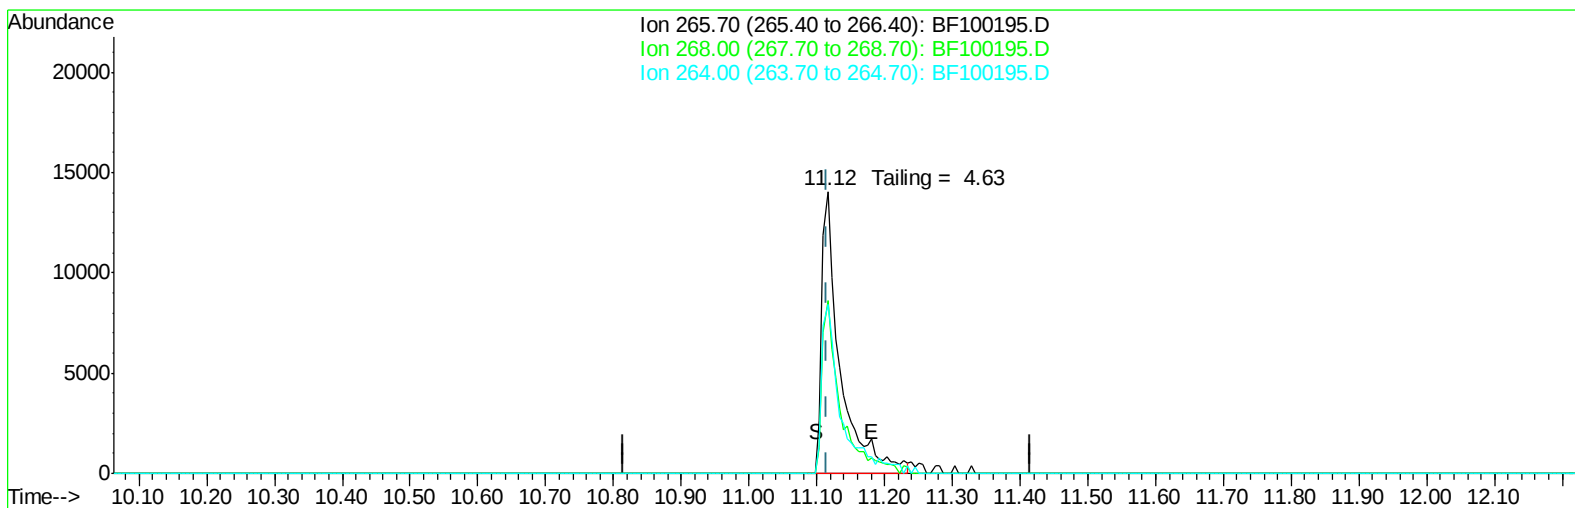

TIC: BF100195.D

(69) Pentachlorophenol (C)




11.116min (+0.000) 51753.20ng

response 25723

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.52
264.00	61.90	60.20
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100195.D
 Acq On : 4 Nov 2017 22:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 04:53:34 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 03 15:46:10 2017
 Response via : Initial Calibration

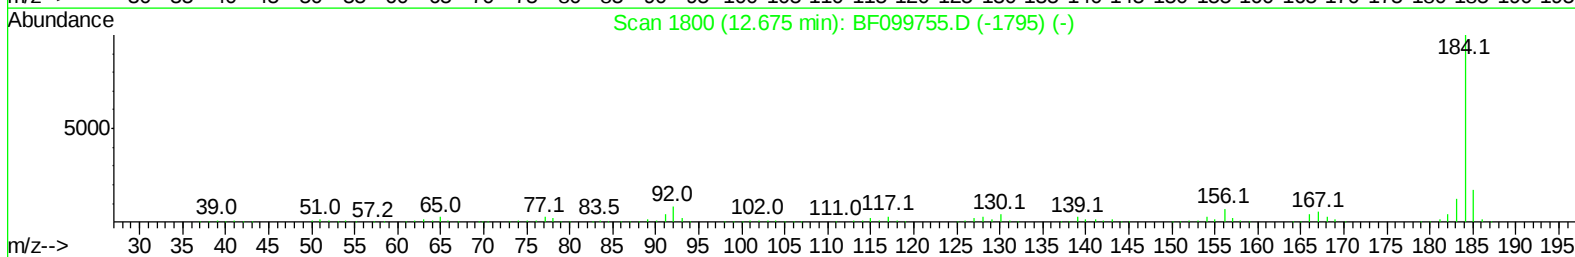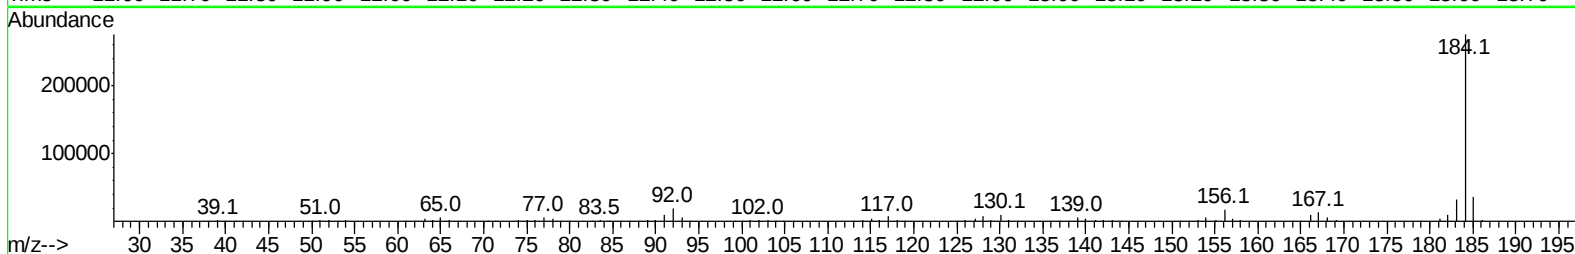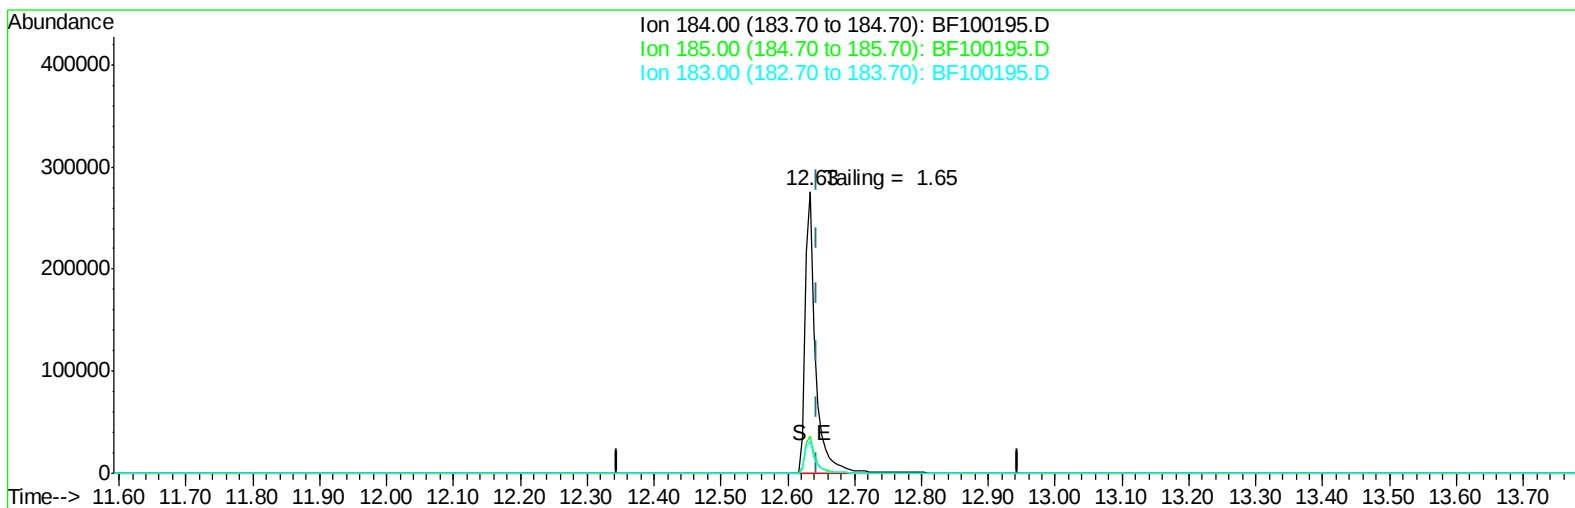

TIC: BF100195.D

(76) Benzidine

12.633min (-0.012) 0.00ng

response 307200

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.32
183.00	11.60	11.59
0.00	0.00	0.00