

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100192.D
 Acq On : 4 Nov 2017 21:24
 Operator : SJ/JU
 Sample : I6313-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PET-BF017-01

Quant Time: Nov 06 02:08:20 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 03 15:46:10 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.76	152	90555	20.00	ng	0.00
21) Naphthalene-d8	8.05	136	376919	20.00	ng	0.00
38) Acenaphthene-d10	9.80	164	179859	20.00	ng	-0.01
63) Phenanthrene-d10	11.29	188	337982	20.00	ng	-0.01
75) Chrysene-d12	13.94	240	226857	20.00	ng	-0.01
86) Perylene-d12	15.40	264	165451	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	672151	116.53	ng	0.00
7) Phenol-d6	6.42	99	806605	117.94	ng	-0.01
23) Nitrobenzene-d5	7.33	82	453976	77.54	ng	-0.02
41) 2,4,6-Tribromophenol	10.60	330	191779	117.00	ng	-0.01
44) 2-Fluorobiphenyl	9.12	172	929374	79.72	ng	-0.01
78) Terphenyl-d14	12.87	244	869022	83.72	ng	-0.01
Target Compounds						
10) Phenol	6.43	94	32453	4.322	ng	Qvalue # 67
49) Dimethylphthalate	9.52	163	100806	7.077	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100192.D
Acq On : 4 Nov 2017 21:24
Operator : SJ/JU
Sample : I6313-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PET-BF017-01

Quant Time: Nov 06 02:08:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:46:10 2017
Response via : Initial Calibration

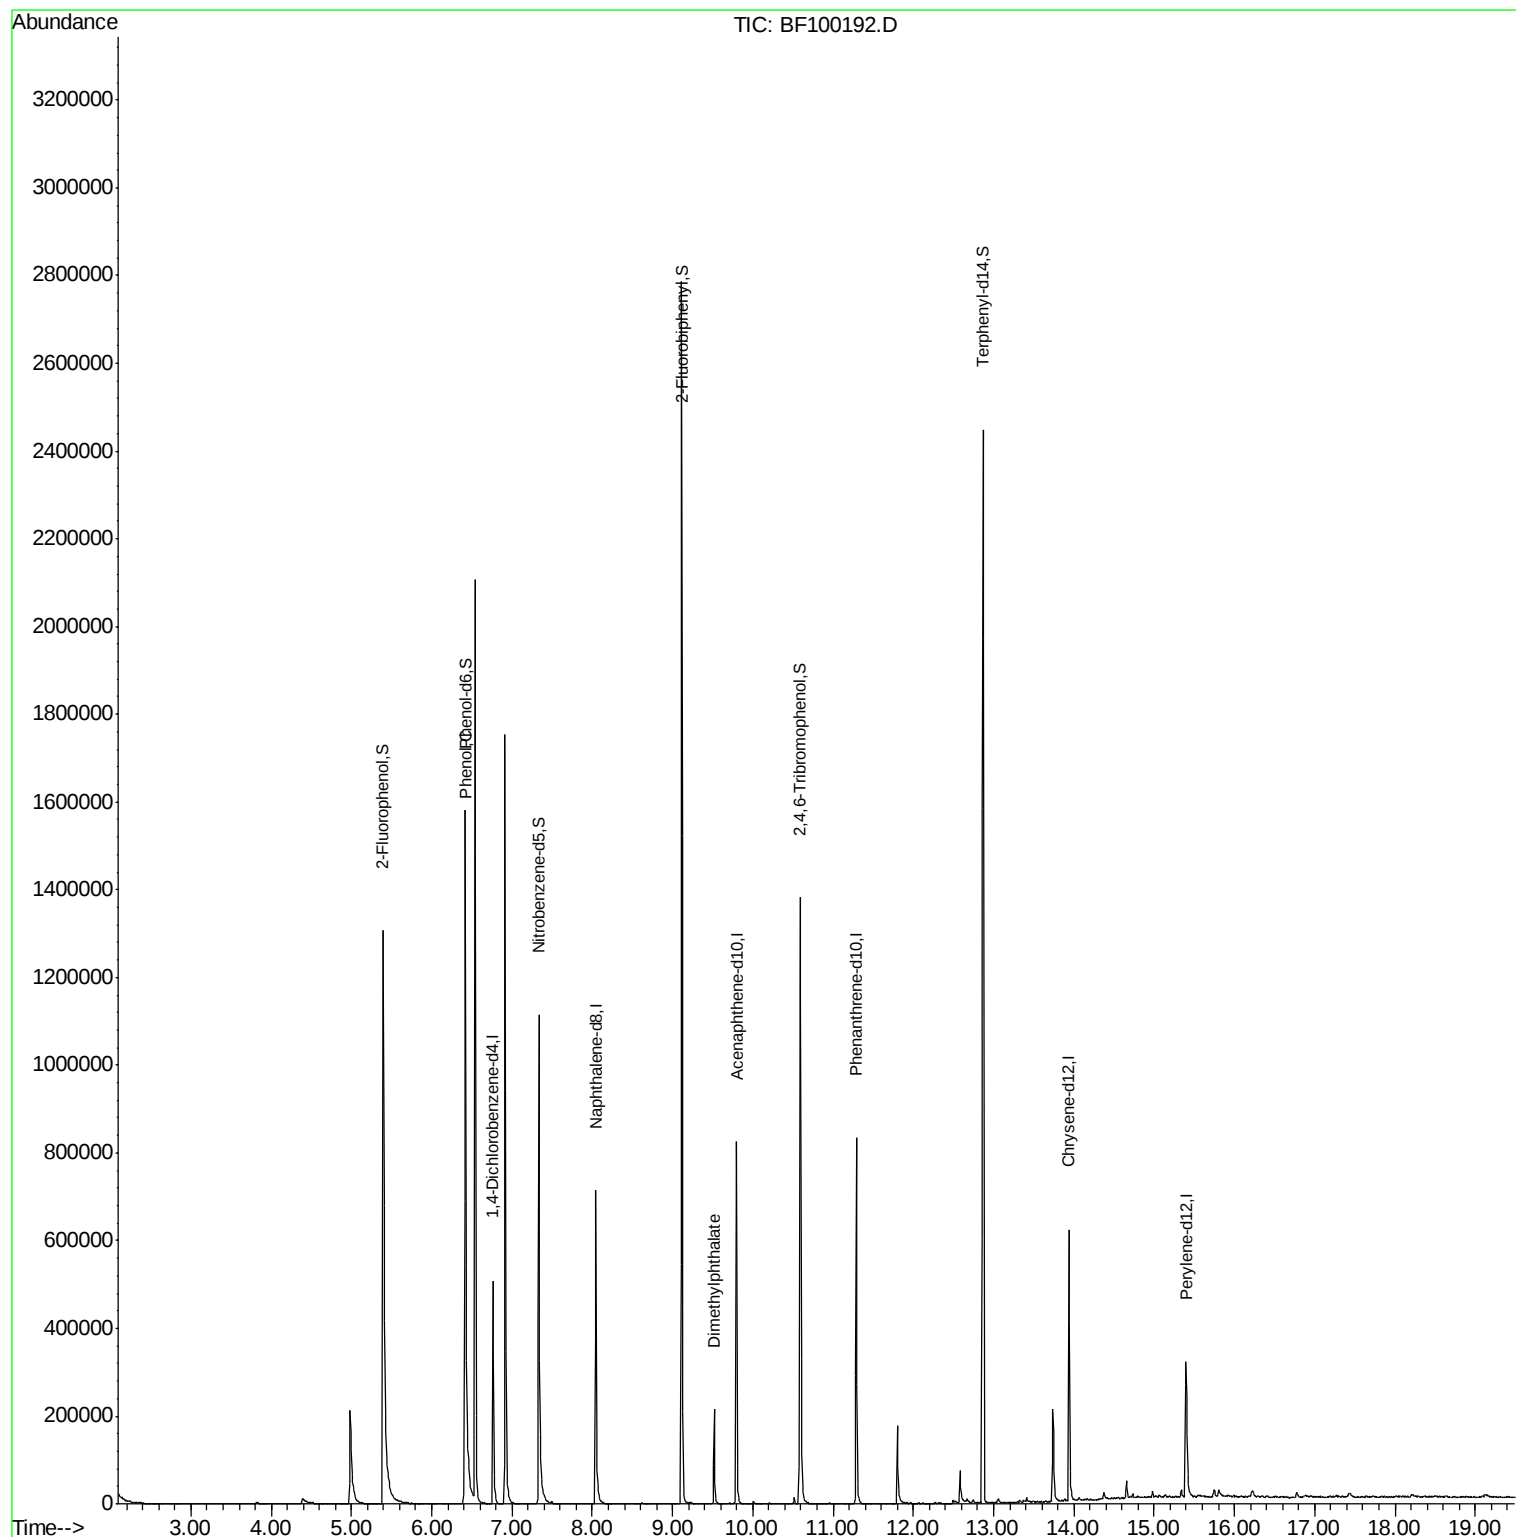

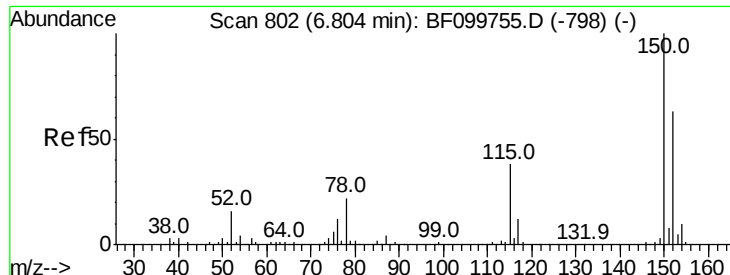


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.76 min Scan# 795
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Instrument :
BNA_F
ClientSampleId :
PET-BF017-01

Tot Ion:152 Resp: 90555
Ion Ratio Lower Upper
152 100
150 154.8 124.6 186.8
115 57.6 50.1 75.1

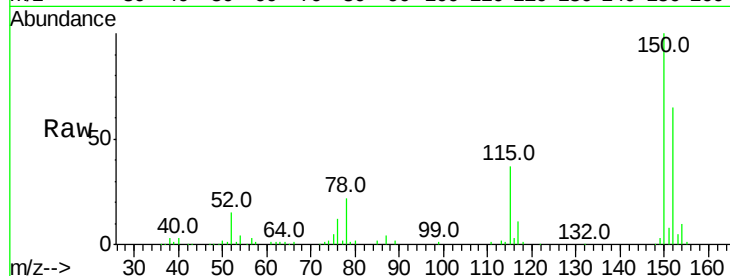


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

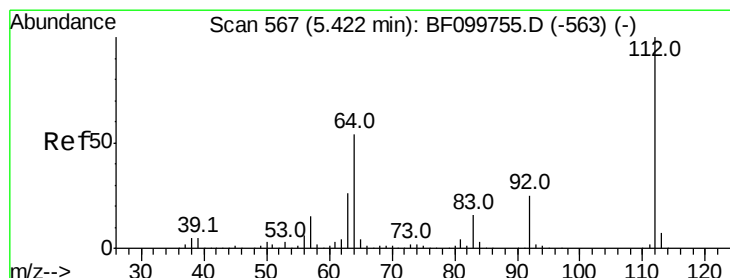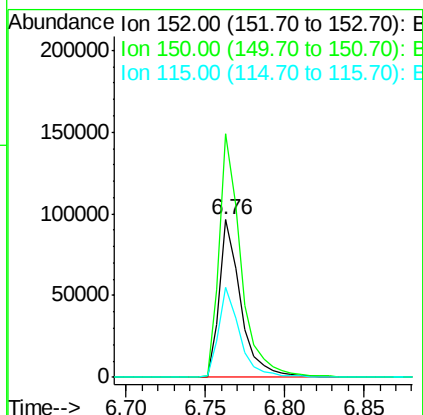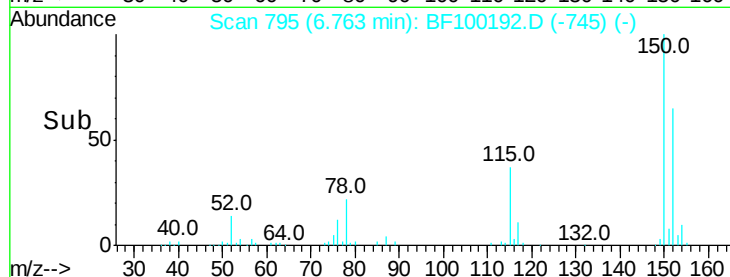



#5


2-Fluorophenol
Concen: 116.532 ng
RT: 5.40 min Scan# 563
Delta R.T. 0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Tgt Ion:112 Resp: 672151
Ion Ratio Lower Upper
112 100
64 47.9 47.9 71.9#
63 23.4 23.7 35.5#

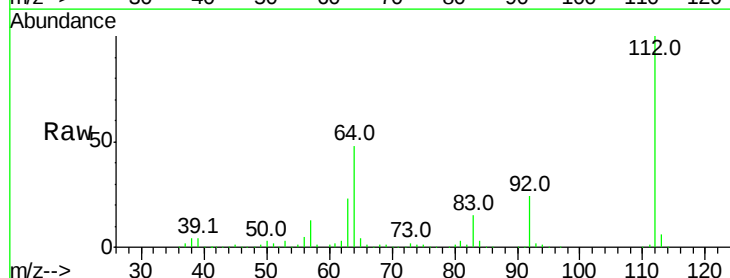

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

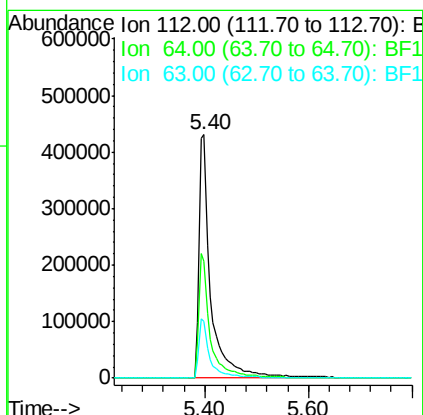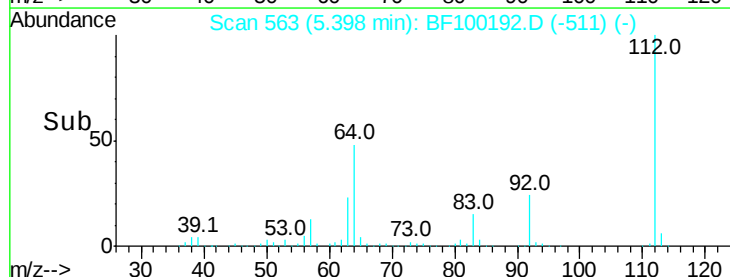

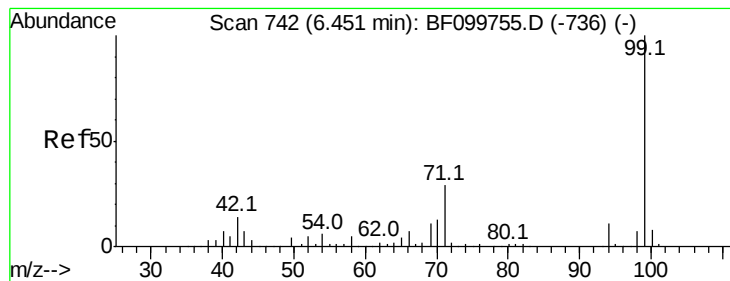

#7

Phenol-d6

Concen: 117.939 ng

RT: 6.42 min Scan# 736

Delta R.T. -0.01 min

Lab File: BF100192.D

Acq: 4 Nov 2017 21:24

Instrument :

BNA_F

ClientSampleId :

PET-BF017-01


Tot Ion: 99 Resp: 806605

Ion Ratio Lower Upper

99 100

42 13.9 14.5 21.7#




71 29.2 25.4 38.0

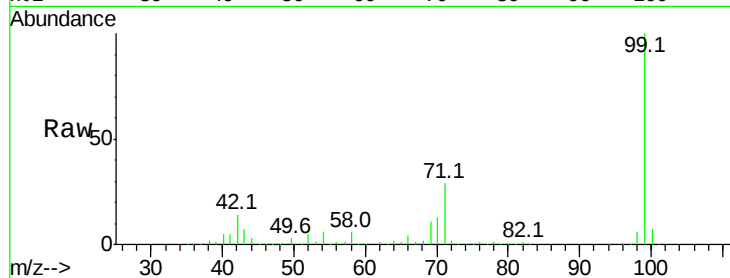

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

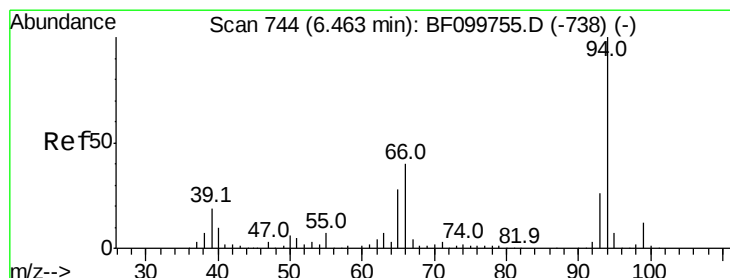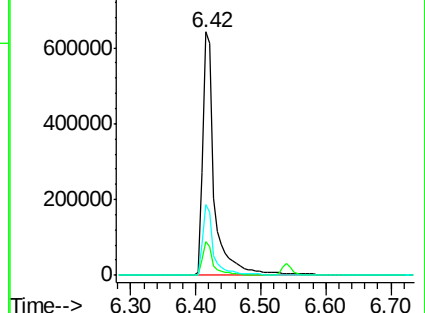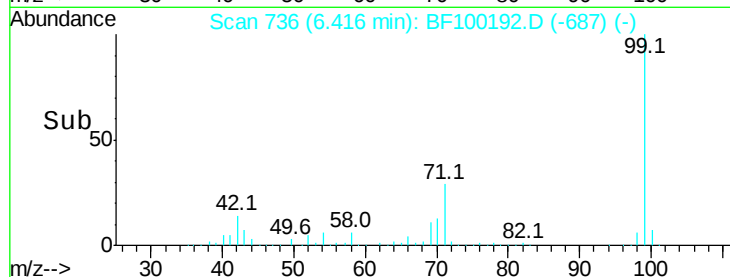

#10

Phenol

Concen: 4.322 ng

RT: 6.43 min Scan# 738

Delta R.T. -0.01 min

Lab File: BF100192.D

Acq: 4 Nov 2017 21:24


Tgt Ion: 94 Resp: 32453

Ion Ratio Lower Upper

94 100

65 31.6 7.9 47.9



66 67.6 16.2 56.2#

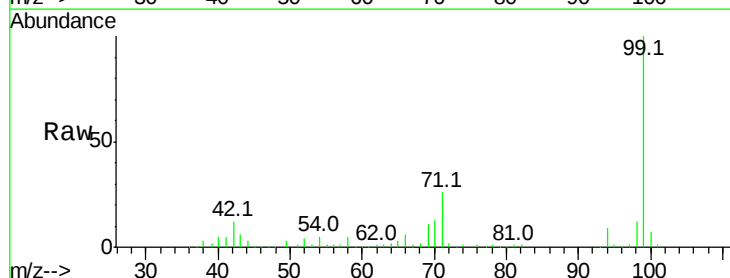


Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

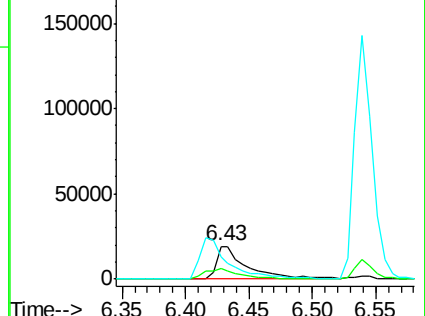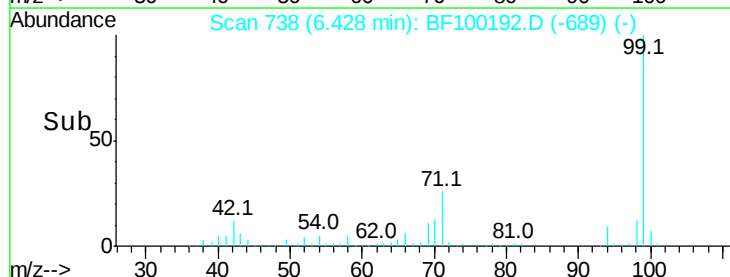

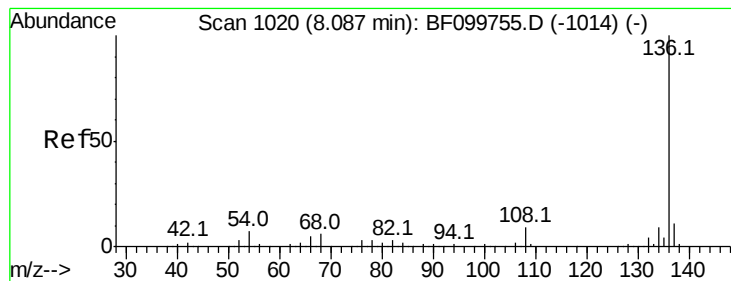

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.05 min Scan# 1013

Delta R.T. -0.01 min

Lab File: BF100192.D

Acq: 4 Nov 2017 21:24

Instrument :

BNA_F

ClientSampleId :

PET-BF017-01

Tot Ion:136 Resp: 376919


Ion Ratio Lower Upper

136 100

137 11.2 8.9 13.3

54 6.4 6.6 9.8#

68 5.8 5.0 7.4



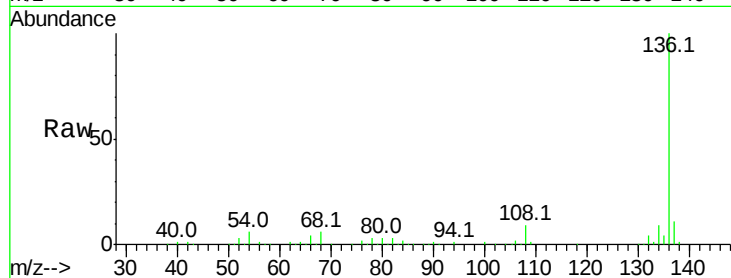


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

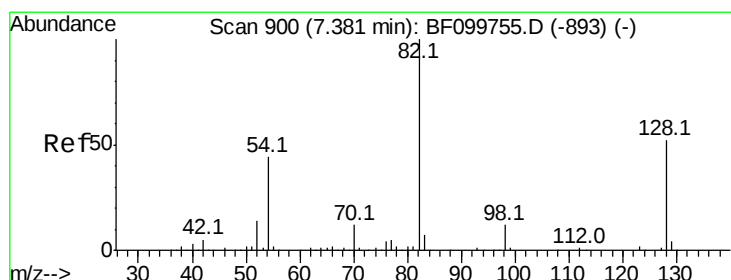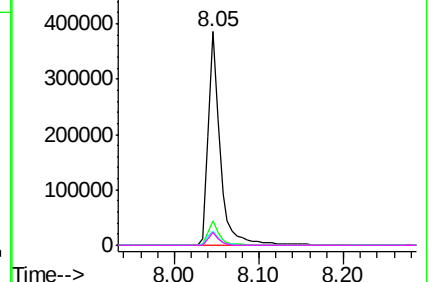

#23

Nitrobenzene-d5

Concen: 77.542 ng

RT: 7.33 min Scan# 892

Delta R.T. -0.02 min

Lab File: BF100192.D

Acq: 4 Nov 2017 21:24


Tgt Ion: 82 Resp: 453976

Ion Ratio Lower Upper

82 100

128 49.7 36.1 54.1



54 43.4 41.4 62.2

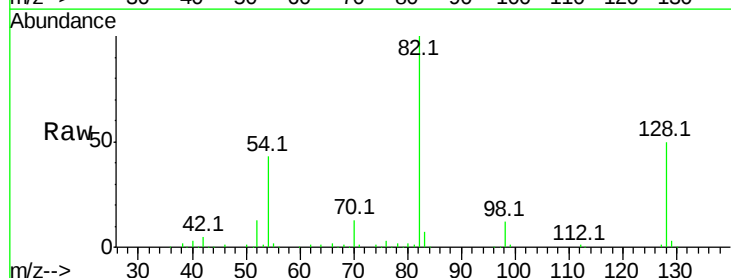


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1



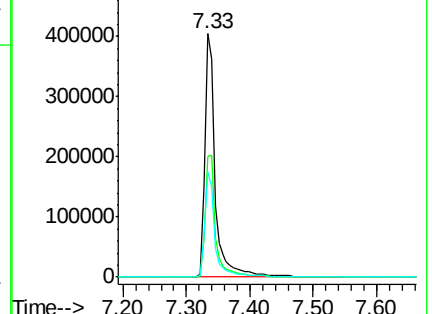





#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.80 min Scan# 1311
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24




Instrument :
BNA_F
ClientSampleId :
PET-BF017-01


Tot Ion:164 Resp: 179859
Ion Ratio Lower Upper
164 100
162 104.7 86.1 129.1
160 47.1 38.3 57.5

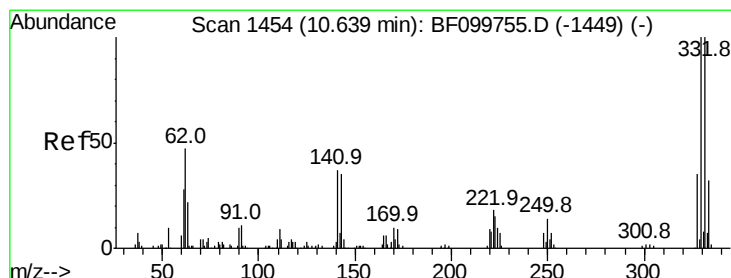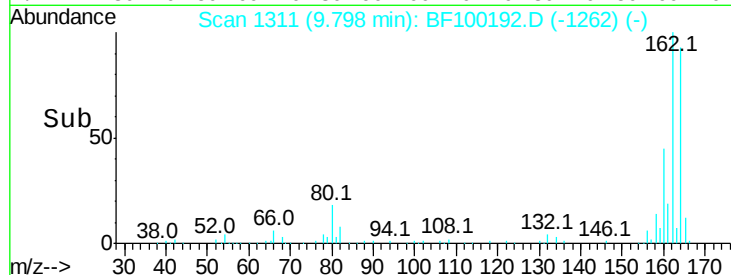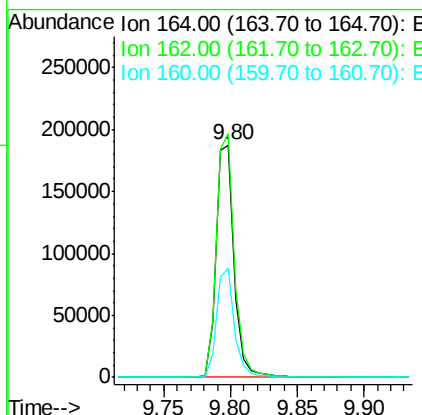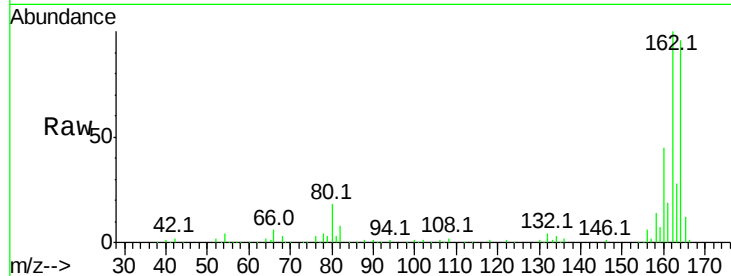

#41
2,4,6-Tribromophenol
Concen: 117.004 ng
RT: 10.60 min Scan# 1447
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Tgt Ion:330 Resp: 191779
Ion Ratio Lower Upper
330 100
332 96.4 77.0 115.6
141 33.9 29.9 44.9



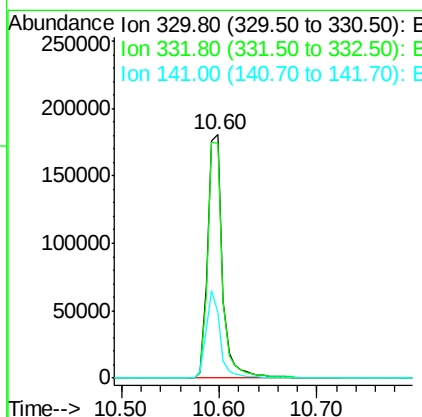
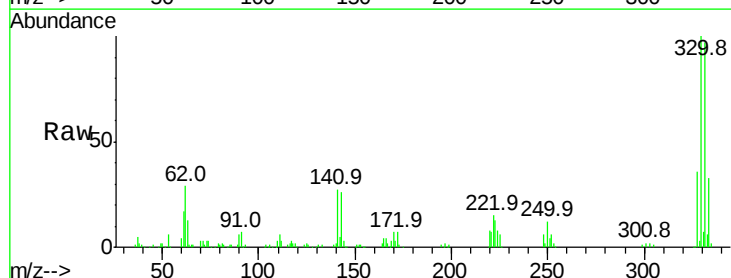




#44
2-Fluorobiphenyl
Concen: 79.722 ng
RT: 9.12 min Scan# 1195
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24




Instrument :
BNA_F
ClientSampleId :
PET-BF017-01


Tot Ion:172 Resp: 929374
Ion Ratio Lower Upper
172 100
171 35.9 29.7 44.5
170 23.3 19.6 29.4

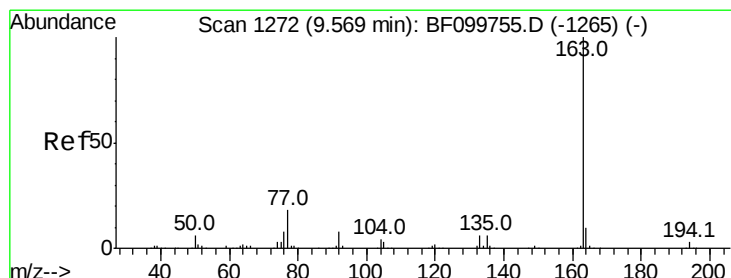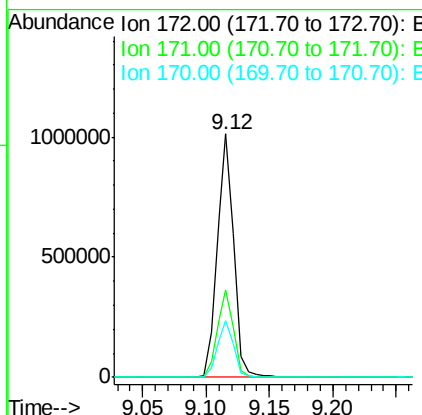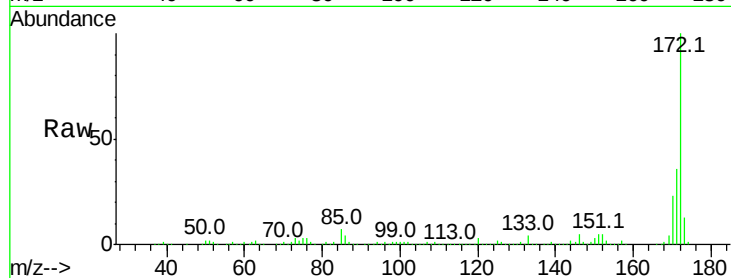

#49
Dimethylphthalate
Concen: 7.077 ng
RT: 9.52 min Scan# 1263
Delta R.T. -0.02 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Tgt Ion:163 Resp: 100806
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 9.6 8.2 12.2

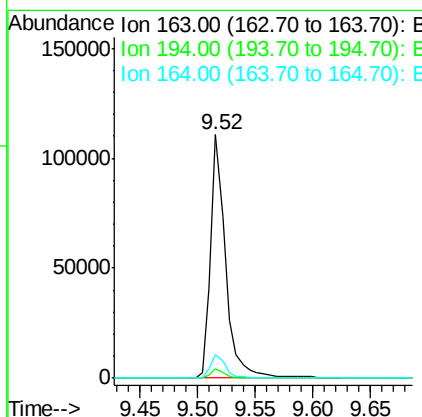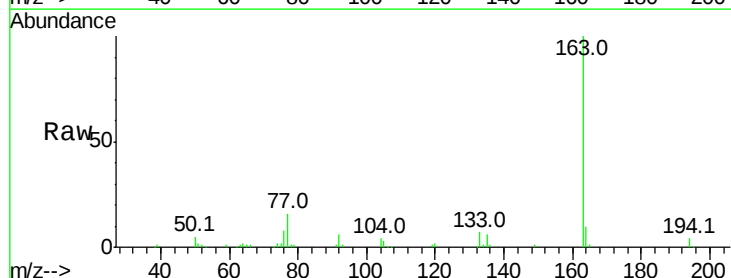







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.29 min Scan# 1564
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Instrument :
BNA_F
ClientSampleId :
PET-BF017-01

Tot Ion:188 Resp: 337982
Ion Ratio Lower Upper
188 100
94 10.4 8.5 12.7
80 11.6 9.2 13.8

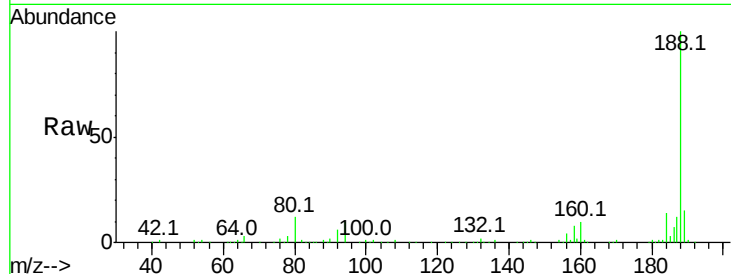


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

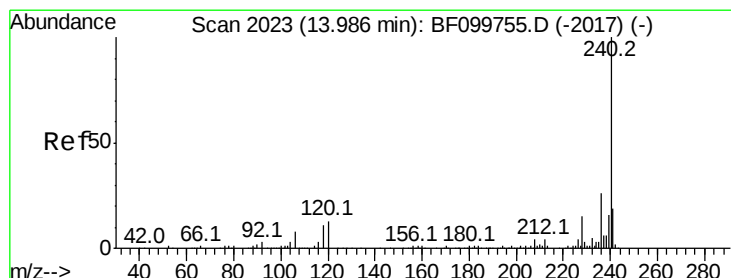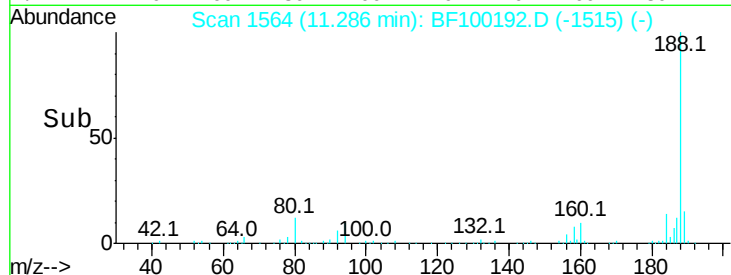
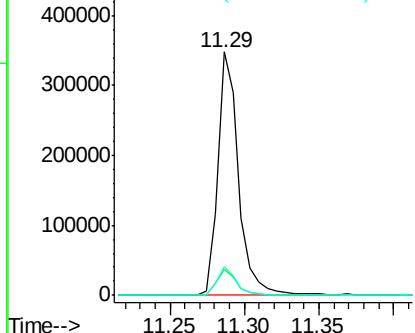



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.94 min Scan# 2015
Delta R.T. -0.01 min
Lab File: BF100192.D
Acq: 4 Nov 2017 21:24

Tgt Ion:240 Resp: 226857
Ion Ratio Lower Upper
240 100
120 13.4 9.5 14.3
236 24.6 20.7 31.1

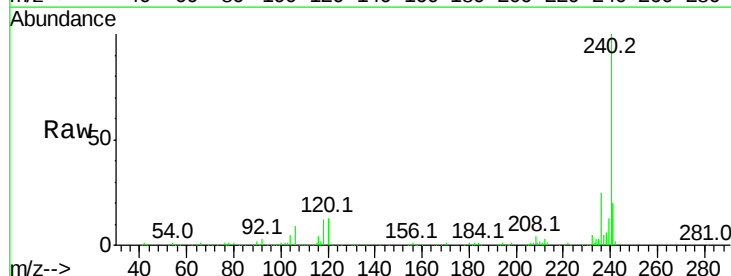

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

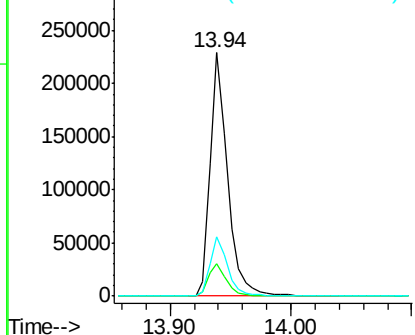


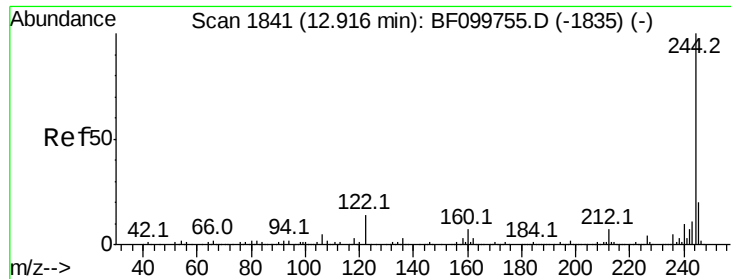




#78
 Terphenyl-d14
 Concen: 83.715 ng
 RT: 12.87 min Scan# 1833
 Delta R.T. -0.01 min
 Lab File: BF100192.D
 Acq: 4 Nov 2017 21:24

Instrument :
 BNA_F
 ClientSampleId :
 PET-BF017-01

Tot Ion:244 Resp: 869022
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.4 8.0
 122 13.9 11.0 16.4

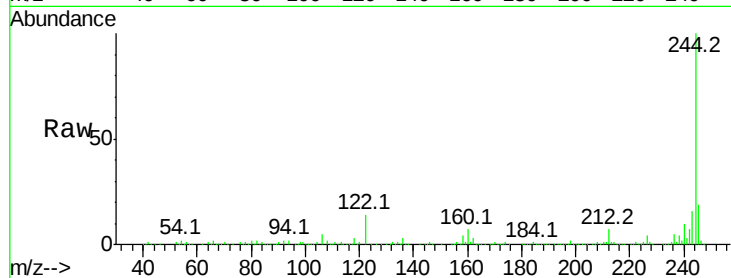


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

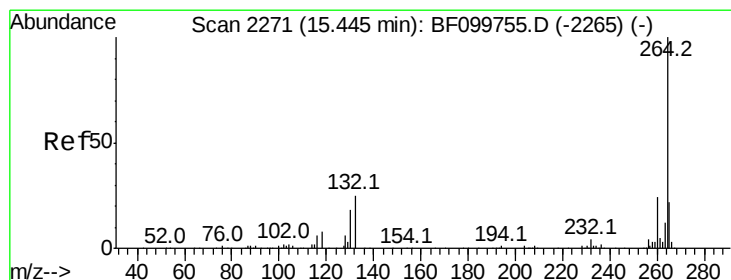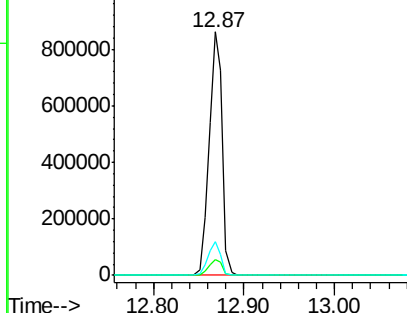

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.40 min Scan# 2263
 Delta R.T. -0.01 min
 Lab File: BF100192.D
 Acq: 4 Nov 2017 21:24

Tgt Ion:264 Resp: 165451
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.2 28.8
 265 20.9 17.5 26.3

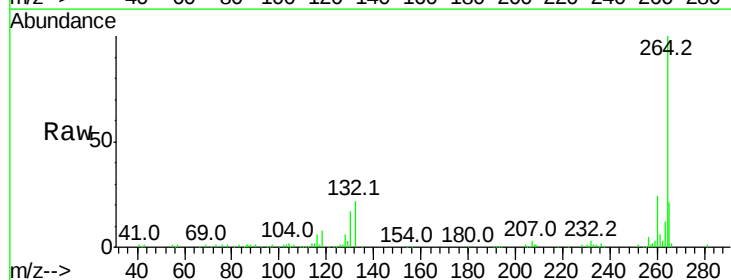

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

