

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
 Data File : BF100202.D
 Acq On : 5 Nov 2017 2:26
 Operator : SJ/JU
 Sample : I6327-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-TIDO-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	491	494	514	rBV	26247	64797	2.46%	0.423%
2	5.404	561	564	602	rBV	258321	623179	23.69%	4.065%
3	6.434	736	739	751	rBV	189296	366286	13.93%	2.389%
4	6.539	754	757	776	rVB	1027616	1315001	50.00%	8.578%
5	6.763	792	795	809	rBV	413482	417940	15.89%	2.726%
6	6.916	818	821	844	rBV	1722665	1663598	63.25%	10.852%
7	7.339	889	893	913	rBV	1137639	1279036	48.63%	8.343%
8	8.045	1010	1013	1036	rBV	560699	601115	22.86%	3.921%
9	9.116	1191	1195	1210	rBV	2847694	2630097	100.00%	17.156%
10	9.798	1304	1311	1325	rBB	749282	755587	28.73%	4.929%
11	10.463	1421	1424	1430	rBB	45255	41229	1.57%	0.269%
12	10.592	1443	1446	1460	rBV	1063726	1084225	41.22%	7.072%
13	11.286	1561	1564	1575	rBV	737550	762516	28.99%	4.974%
14	12.668	1796	1799	1802	rBV	66405	49051	1.86%	0.320%
15	12.868	1829	1833	1836	rBV	2578108	2628479	99.94%	17.146%
16	13.374	1915	1919	1923	rBV	42222	35626	1.35%	0.232%
17	13.745	1978	1982	1988	rBV	23849	28467	1.08%	0.186%
18	13.939	2012	2015	2028	rVB	547132	588820	22.39%	3.841%
19	15.398	2259	2263	2279	rBV	241930	395178	15.03%	2.578%


Sum of corrected areas: 15330227

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100202.D
Acq On : 5 Nov 2017 2:26
Operator : SJ/JU
Sample : I6327-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

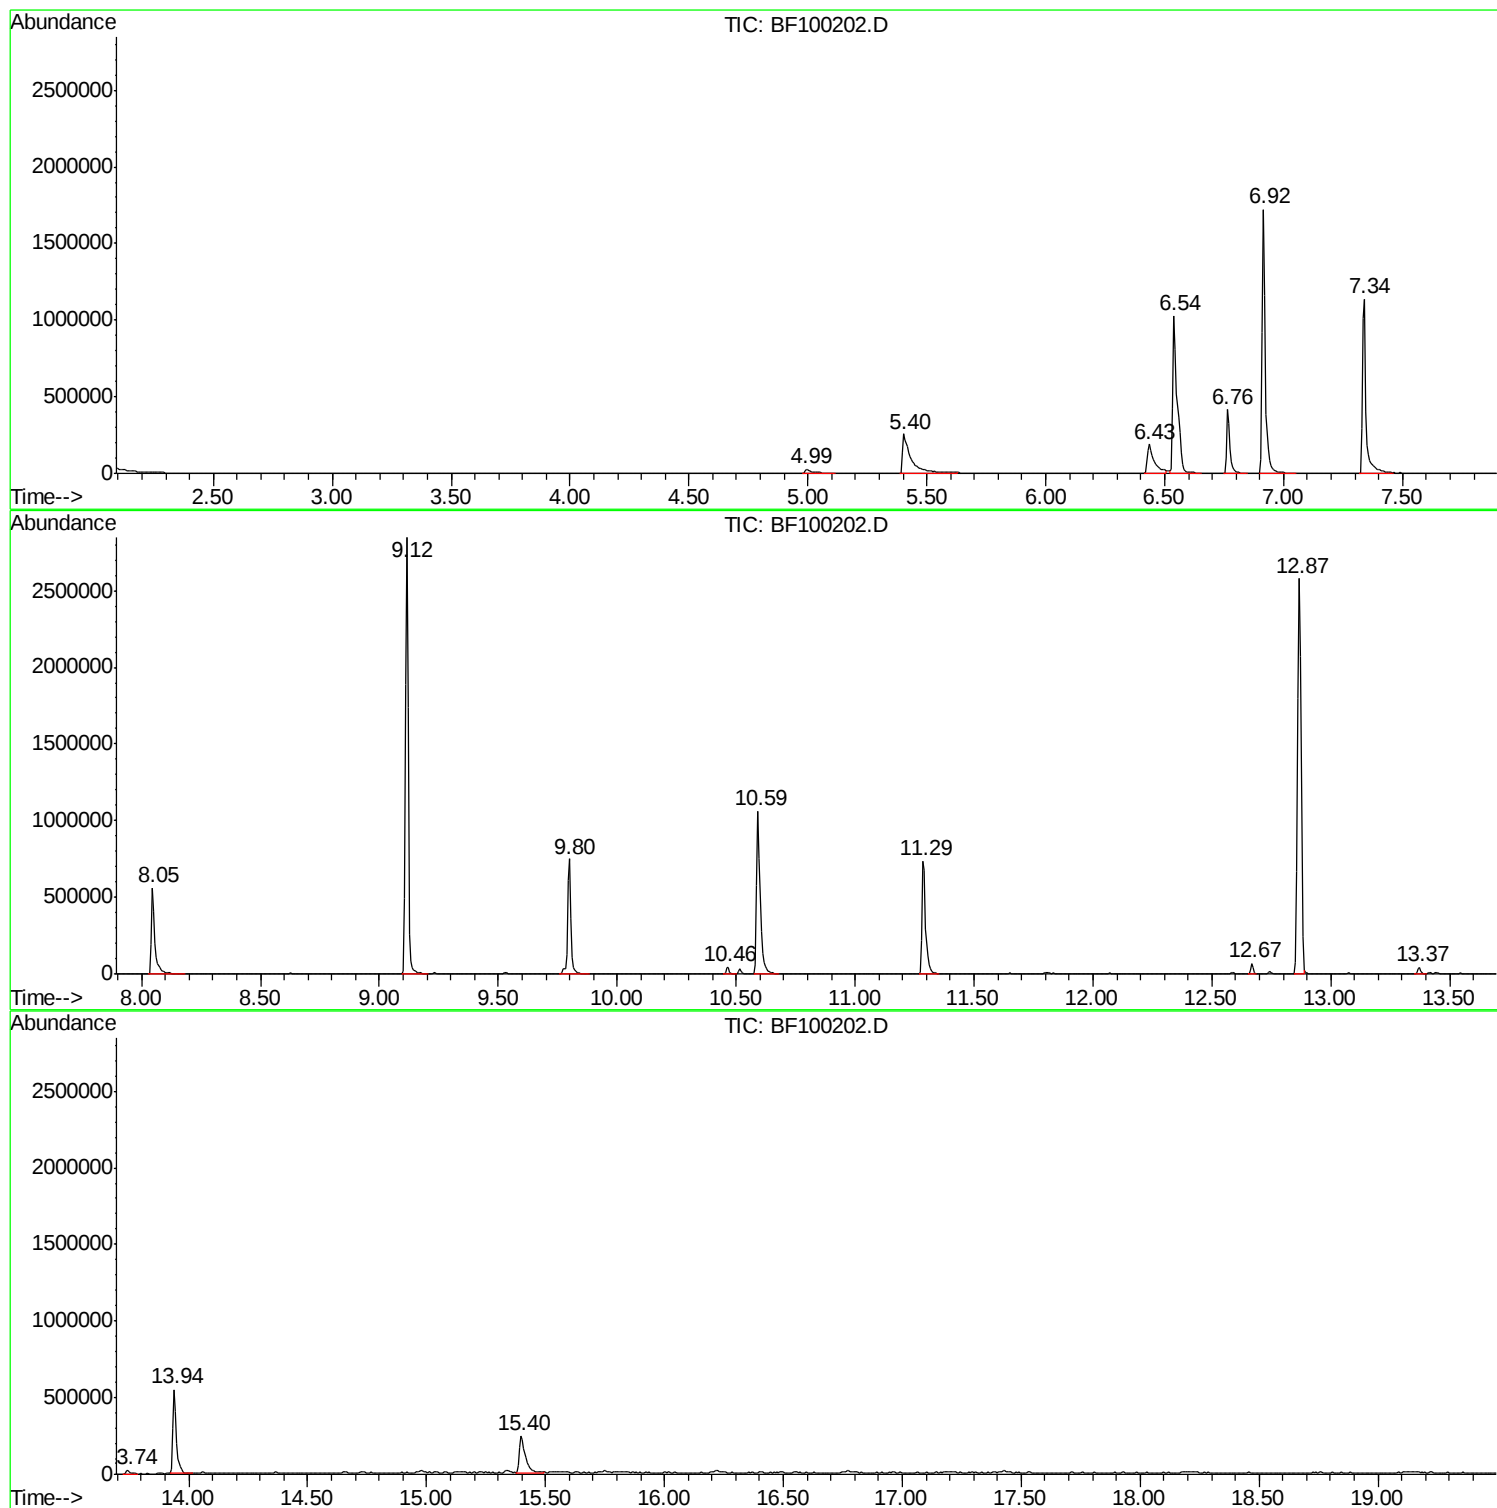

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100202.D
Acq_On : 5-Nov-2017 2:266
Operator : SJ/JUU
Sample : I6327-011
Misc :
ALS_Vial : 31 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
