

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100204.D
 Acq On : 5 Nov 2017 3:19
 Operator : SJ/JU
 Sample : I6327-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-TIDO-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	491	493	510	rBV	58157	117209	4.03%	0.681%
2	5.404	561	564	592	rBV	310352	691381	23.79%	4.019%
3	6.428	736	738	754	rBV	255551	475226	16.35%	2.762%
4	6.540	754	757	776	rVB	1245947	1505352	51.80%	8.750%
5	6.763	792	795	810	rBV	513069	501437	17.26%	2.915%
6	6.916	818	821	839	rBV	2011222	1916626	65.95%	11.140%
7	7.340	889	893	913	rBV	1431469	1492502	51.36%	8.675%
8	8.045	1010	1013	1027	rBV	687323	703513	24.21%	4.089%
9	9.116	1191	1195	1198	rBV	3079814	2905978	100.00%	16.891%
10	9.798	1302	1311	1324	rBV	875747	877327	30.19%	5.099%
11	10.463	1421	1424	1430	rBB	50482	44404	1.53%	0.258%
12	10.516	1430	1433	1440	rBB	44711	40164	1.38%	0.233%
13	10.592	1443	1446	1460	rBV	1174389	1181034	40.64%	6.865%
14	11.286	1561	1564	1575	rVB	818866	837669	28.83%	4.869%
15	12.869	1829	1833	1837	rBV	2619681	2795358	96.19%	16.248%
16	13.739	1978	1981	1988	rBV	48877	58464	2.01%	0.340%
17	13.939	2012	2015	2028	rBV	592957	641702	22.08%	3.730%
18	15.398	2259	2263	2279	rBV	270313	419094	14.42%	2.436%


Sum of corrected areas: 17204440

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100204.D
Acq On : 5 Nov 2017 3:19
Operator : SJ/JU
Sample : I6327-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

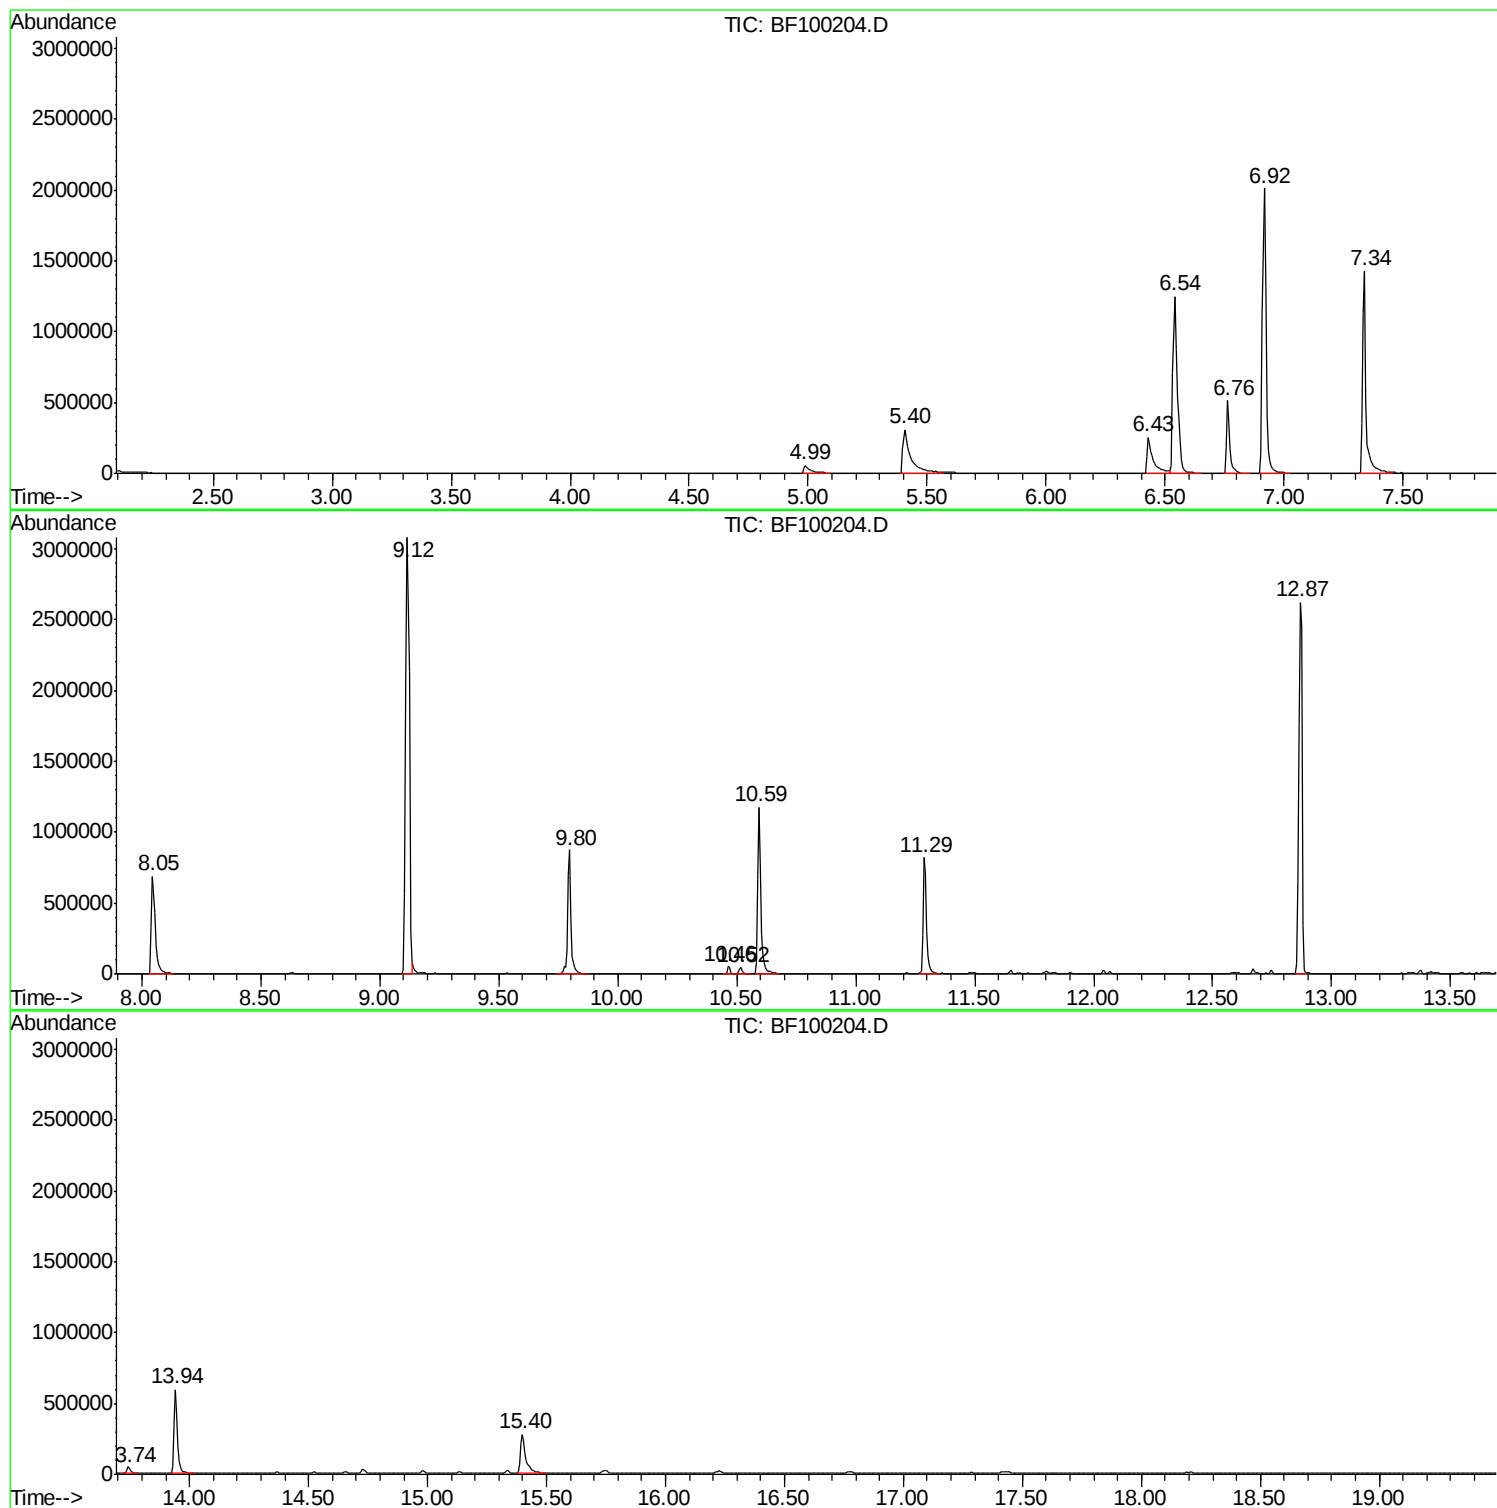

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100204.D
Acq_On : 5-Nov-2017 3:199
Operator : SJ/JUU
Sample : I6327-033
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-U-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
