

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100205.D
 Acq On : 5 Nov 2017 3:46
 Operator : SJ/JU
 Sample : I6327-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-TIDO-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	491	494	510	rBV	33481	76517	2.66%	0.467%
2	5.404	562	564	590	rBV	259885	600086	20.88%	3.665%
3	6.428	736	738	754	rBV	189359	394708	13.73%	2.411%
4	6.540	754	757	774	rVB	1128980	1409268	49.02%	8.607%
5	6.763	792	795	809	rVB	502089	494768	17.21%	3.022%
6	6.916	818	821	842	rBV	1959351	1864213	64.85%	11.385%
7	7.340	889	893	912	rBV	1313613	1430180	49.75%	8.734%
8	8.045	1010	1013	1032	rBV	676091	707255	24.60%	4.319%
9	9.116	1191	1195	1205	rBV	3010571	2874618	100.00%	17.556%
10	9.798	1302	1311	1324	rBV	902808	872366	30.35%	5.328%
11	10.469	1421	1425	1430	rBV	43805	40953	1.42%	0.250%
12	10.516	1430	1433	1439	rVB	51271	43900	1.53%	0.268%
13	10.592	1443	1446	1460	rBV	1105898	1121293	39.01%	6.848%
14	11.286	1561	1564	1575	rBV	799028	842606	29.31%	5.146%
15	12.869	1829	1833	1836	rBV	2571431	2613138	90.90%	15.959%
16	13.939	2012	2015	2026	rBV	580683	592270	20.60%	3.617%
17	15.398	2260	2263	2277	rBV2	256185	396170	13.78%	2.419%


Sum of corrected areas: 16374309

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100205.D
Acq On : 5 Nov 2017 3:46
Operator : SJ/JU
Sample : I6327-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

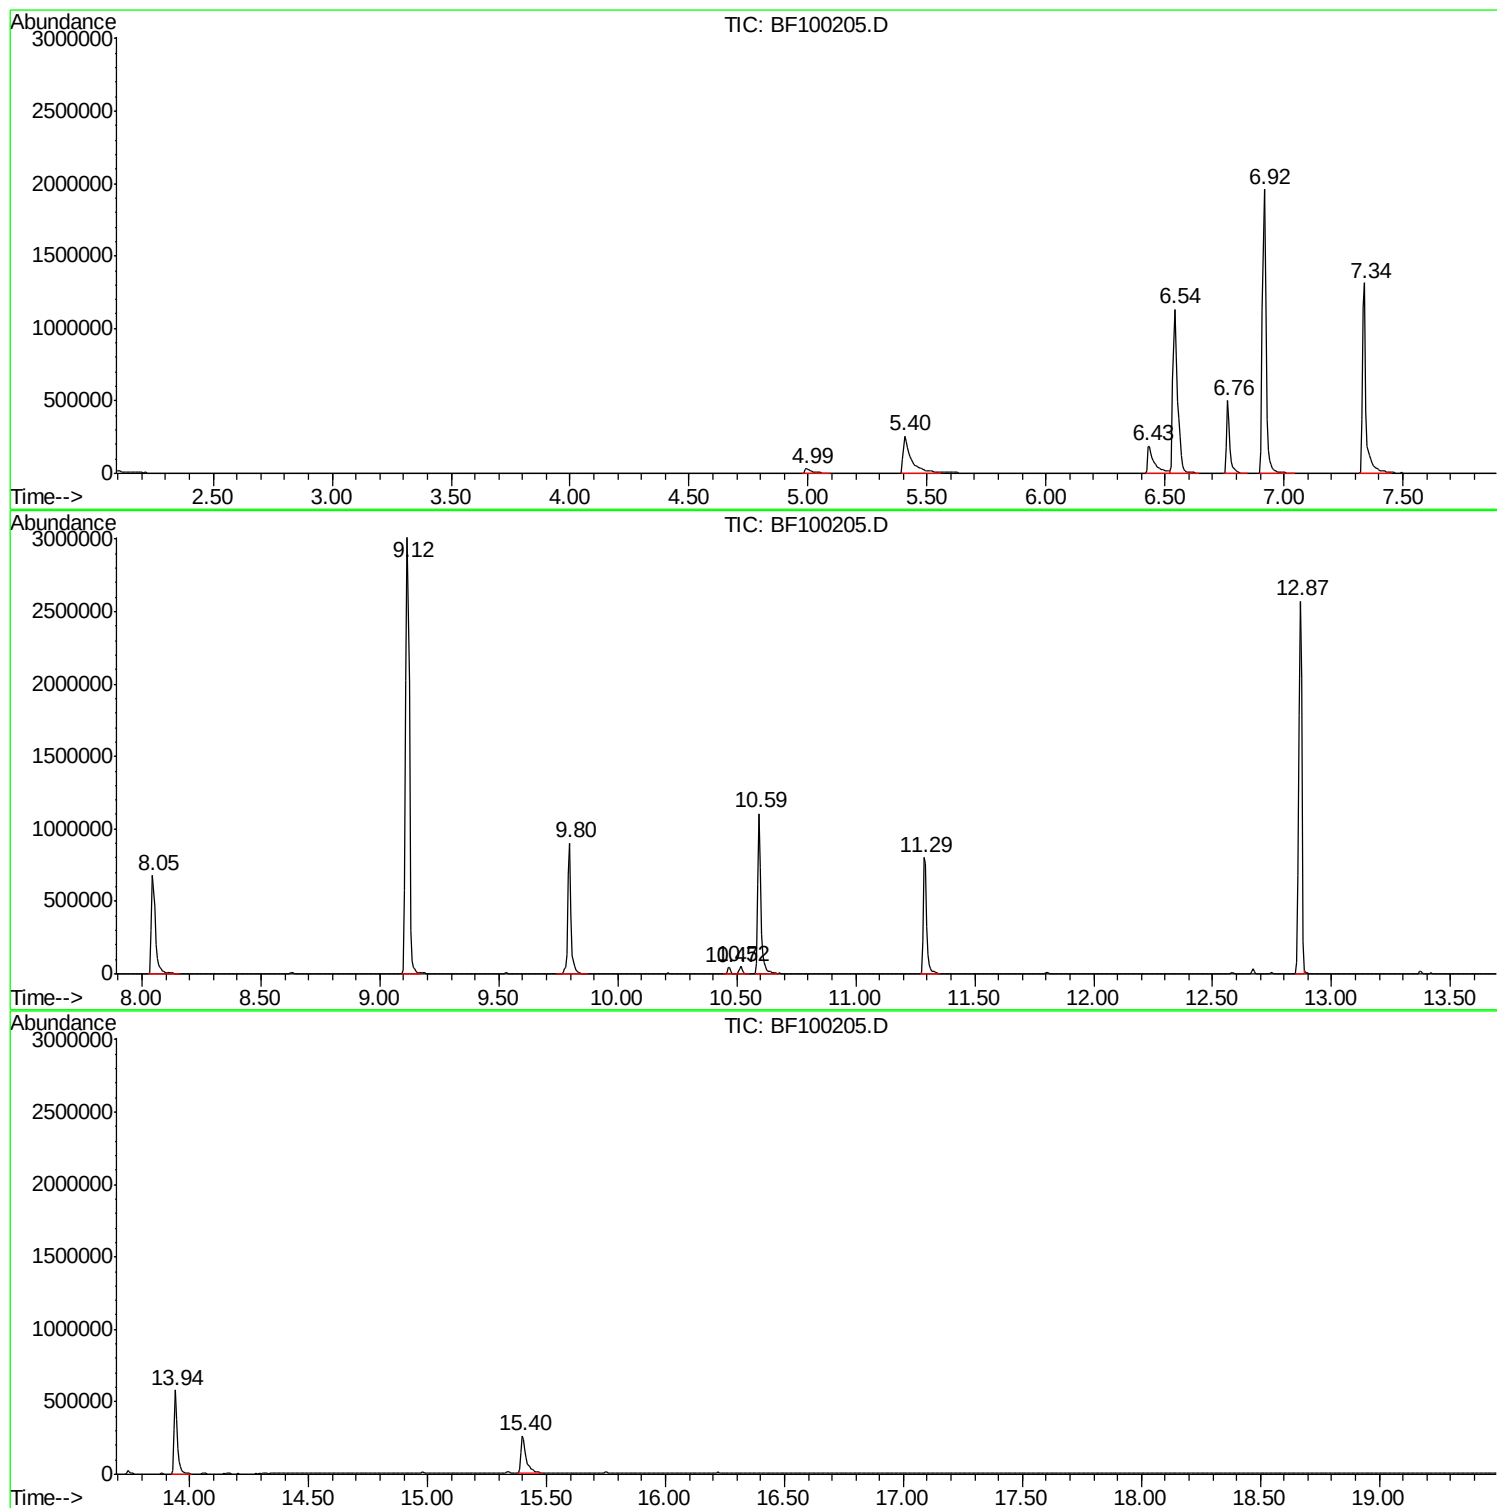

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100205.D
Acq_On : 5-Nov-2017 3:466
Operator : SJ/JUU
Sample : I6327-044
Misc :
ALS_Vial : 34 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-TIDO-F-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
