

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
 Data File : BF100206.D
 Acq On : 5 Nov 2017 4:12
 Operator : SJ/JU
 Sample : I6327-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-JETT-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	505	rBV	42486	85117	3.23%	0.548%
2	5.404	562	564	600	rBV	269611	640407	24.29%	4.126%
3	6.428	736	738	754	rBV	228822	444763	16.87%	2.866%
4	6.539	754	757	781	rVB	1116470	1377071	52.24%	8.873%
5	6.763	793	795	810	rVB	458608	453498	17.20%	2.922%
6	6.916	818	821	840	rBV	1841320	1782428	67.62%	11.484%
7	7.339	889	893	917	rBV	1183267	1369488	51.95%	8.824%
8	8.045	1010	1013	1033	rBV	600284	638043	24.21%	4.111%
9	9.116	1191	1195	1198	rBV	2987150	2635982	100.00%	16.984%
10	9.798	1304	1311	1325	rBB	738069	774910	29.40%	4.993%
11	10.463	1421	1424	1430	rBV	56390	49685	1.88%	0.320%
12	10.516	1430	1433	1440	rVB	48148	42757	1.62%	0.275%
13	10.592	1443	1446	1459	rBV	1030747	1034405	39.24%	6.665%
14	11.292	1561	1565	1576	rBV	674558	743002	28.19%	4.787%
15	12.868	1829	1833	1836	rBV	2586535	2509285	95.19%	16.168%
16	13.739	1978	1981	1987	rBV2	46528	55202	2.09%	0.356%
17	13.939	2012	2015	2023	rBV	495325	526758	19.98%	3.394%
18	15.398	2260	2263	2272	rBV	223431	357679	13.57%	2.305%


Sum of corrected areas: 15520480

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100206.D
Acq On : 5 Nov 2017 4:12
Operator : SJ/JU
Sample : I6327-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

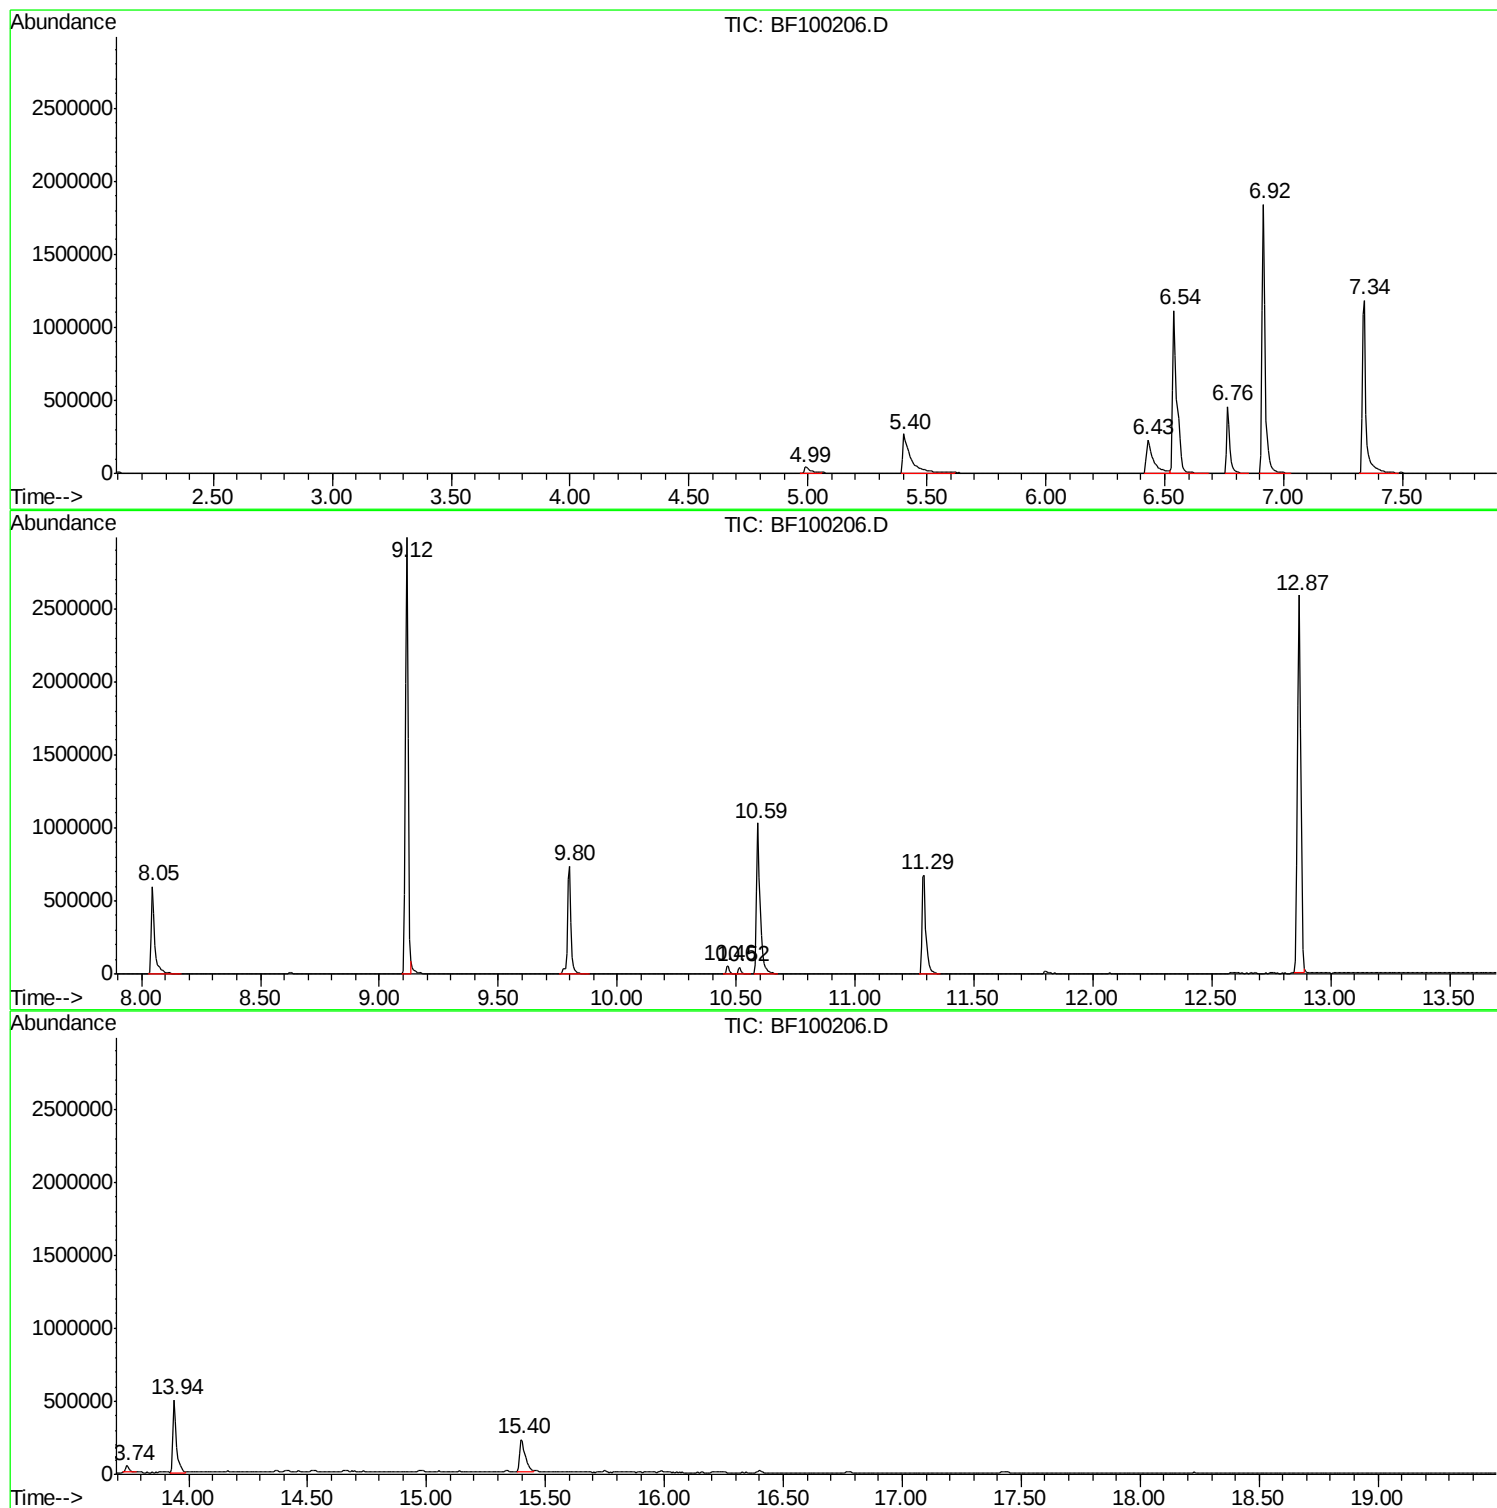

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100206.D
Acq_On : 5-Nov-2017 4:122
Operator : SJ/JUU
Sample : I6327-055
Misc :
ALS_Vial : 35 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-D-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
