

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
 Data File : BF100207.D
 Acq On : 5 Nov 2017 4:39
 Operator : SJ/JU
 Sample : I6327-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-JETT-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	491	494	508	rBV2	35750	82457	3.13%	0.528%
2	5.404	562	564	591	rBV	241548	592981	22.48%	3.798%
3	6.428	736	738	754	rBV	208478	413690	15.68%	2.650%
4	6.540	754	757	781	rVB	1073104	1335666	50.64%	8.554%
5	6.763	792	795	810	rBB	457901	464284	17.60%	2.974%
6	6.916	818	821	841	rBV	1843346	1752514	66.44%	11.224%
7	7.339	889	893	917	rBV	1192215	1346409	51.05%	8.623%
8	8.045	1010	1013	1032	rBV	614172	659910	25.02%	4.226%
9	9.116	1191	1195	1198	rBV	2963886	2637552	100.00%	16.893%
10	9.798	1304	1311	1325	rBB	774228	790205	29.96%	5.061%
11	10.463	1422	1424	1430	rBV	39900	35282	1.34%	0.226%
12	10.516	1430	1433	1440	rVB	52579	44876	1.70%	0.287%
13	10.592	1443	1446	1460	rBV	1025867	1017468	38.58%	6.517%
14	11.286	1561	1564	1576	rBV	758529	777032	29.46%	4.977%
15	12.669	1796	1799	1802	rBV	98364	75910	2.88%	0.486%
16	12.868	1829	1833	1836	rBV	2528700	2552499	96.78%	16.348%
17	13.374	1915	1919	1922	rBV	63705	54111	2.05%	0.347%
18	13.745	1978	1982	1988	rBV	28064	32062	1.22%	0.205%
19	13.939	2012	2015	2027	rBV	519717	563638	21.37%	3.610%
20	15.398	2259	2263	2276	rBV	243573	385093	14.60%	2.466%


Sum of corrected areas: 15613639

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100207.D
Acq On : 5 Nov 2017 4:39
Operator : SJ/JU
Sample : I6327-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

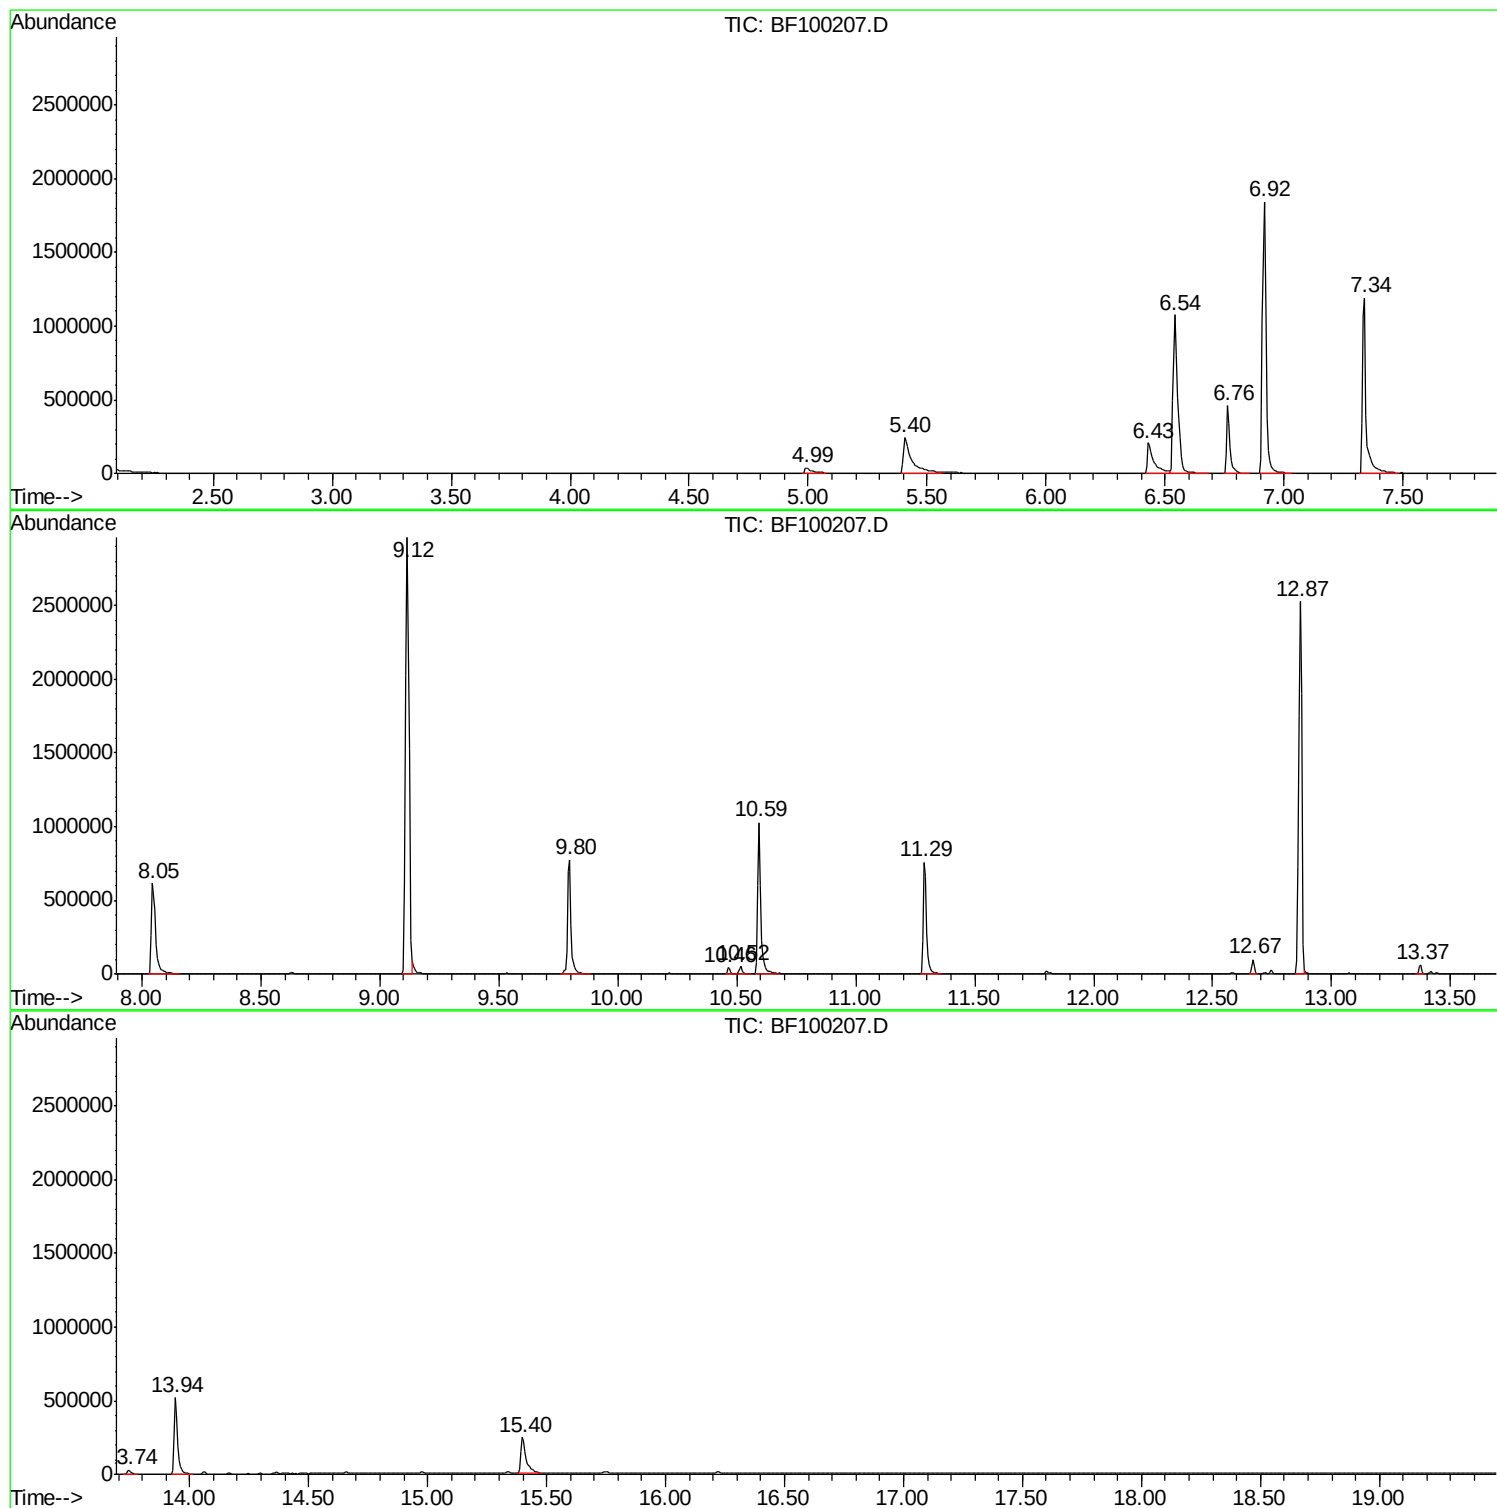

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100207.D
Acq_On : 5-Nov-2017 4:399
Operator : SJ/JUU
Sample : I6327-066
Misc :
ALS_Vial : 36 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
