

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
 Data File : BF100208.D
 Acq On : 5 Nov 2017 5:05
 Operator : SJ/JU
 Sample : I6327-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-JETT-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	491	493	512	rBV	44096	98495	3.57%	0.597%
2	5.404	561	564	590	rBV	285097	649876	23.55%	3.940%
3	6.428	736	738	754	rBV	218977	424284	15.37%	2.572%
4	6.539	754	757	779	rVB	1168996	1441327	52.22%	8.738%
5	6.763	792	795	807	rVB	491106	487431	17.66%	2.955%
6	6.916	818	821	842	rBV	1950275	1857624	67.31%	11.262%
7	7.339	889	893	917	rBV	1264543	1444009	52.32%	8.754%
8	8.045	1010	1013	1028	rBV	666957	691167	25.04%	4.190%
9	9.116	1191	1195	1198	rBV	3075258	2759859	100.00%	16.731%
10	9.798	1304	1311	1327	rBB	835949	854601	30.97%	5.181%
11	10.469	1422	1425	1430	rBV	48728	41383	1.50%	0.251%
12	10.516	1430	1433	1441	rVB	53575	48985	1.77%	0.297%
13	10.592	1443	1446	1461	rBV	1074105	1105564	40.06%	6.702%
14	11.286	1561	1564	1576	rBV	763327	817149	29.61%	4.954%
15	12.668	1796	1799	1802	rBV	136297	101515	3.68%	0.615%
16	12.868	1829	1833	1836	rBV	2638844	2602249	94.29%	15.776%
17	13.368	1915	1918	1922	rBV	78517	68851	2.49%	0.417%
18	13.739	1978	1981	1989	rBV2	40122	46481	1.68%	0.282%
19	13.939	2012	2015	2026	rBV	524243	561772	20.36%	3.406%
20	15.398	2259	2263	2281	rBV	240183	392563	14.22%	2.380%


Sum of corrected areas: 16495185

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100208.D
Acq On : 5 Nov 2017 5:05
Operator : SJ/JU
Sample : I6327-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

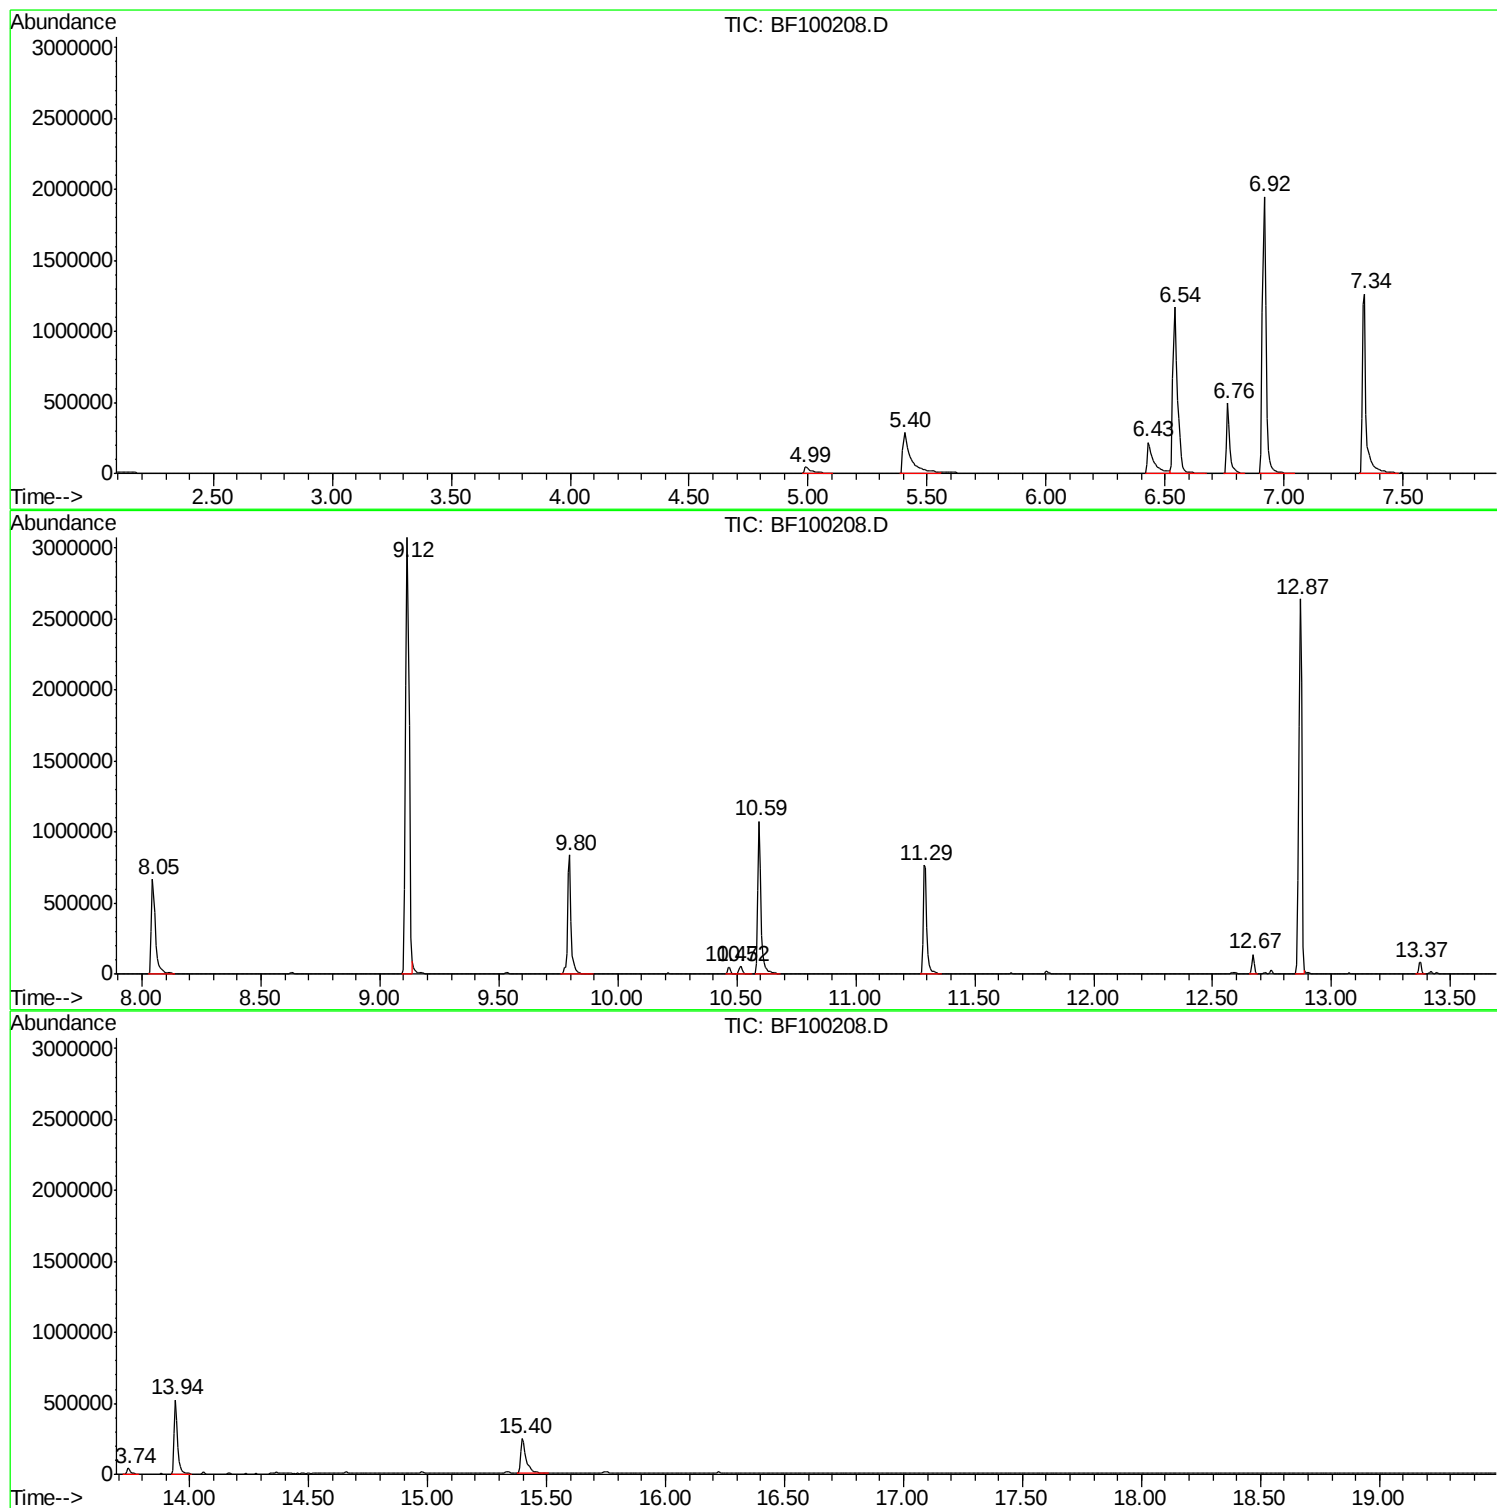

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100208.D
Acq_On : 5-Nov-2017 5:055
Operator : SJ/JUU
Sample : I6327-077
Misc :
ALS_Vial : 37 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-U-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
