

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
 Data File : BF100209.D
 Acq On : 5 Nov 2017 5:32
 Operator : SJ/JU
 Sample : I6327-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-JETT-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	512	rBV	53890	115487	4.04%	0.674%
2	5.404	561	564	592	rBV	305571	704876	24.65%	4.115%
3	6.428	736	738	754	rBV	241152	455897	15.95%	2.662%
4	6.540	754	757	773	rVB	1245524	1513563	52.94%	8.836%
5	6.763	792	795	809	rVB	517570	515707	18.04%	3.011%
6	6.916	818	821	842	rBV	1976425	1897864	66.38%	11.080%
7	7.339	889	893	917	rBV	1377853	1516447	53.04%	8.853%
8	8.045	1010	1013	1029	rBV	698008	726240	25.40%	4.240%
9	9.116	1191	1195	1198	rBV	3179228	2859011	100.00%	16.691%
10	9.798	1304	1311	1323	rBV	828444	882812	30.88%	5.154%
11	10.469	1421	1425	1430	rBB	36125	33820	1.18%	0.197%
12	10.516	1430	1433	1440	rBB	56404	50695	1.77%	0.296%
13	10.592	1443	1446	1460	rBV	1156981	1165267	40.76%	6.803%
14	11.286	1561	1564	1575	rVB	809429	846470	29.61%	4.942%
15	11.798	1645	1651	1656	rBV2	20442	32035	1.12%	0.187%
16	12.869	1829	1833	1836	rBV	2703291	2748632	96.14%	16.046%
17	13.739	1973	1981	1989	rBV3	27656	40519	1.42%	0.237%
18	13.939	2012	2015	2029	rBV	577986	607836	21.26%	3.549%
19	15.398	2259	2263	2274	rBV2	257385	416081	14.55%	2.429%


Sum of corrected areas: 17129259

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100209.D
Acq On : 5 Nov 2017 5:32
Operator : SJ/JU
Sample : I6327-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

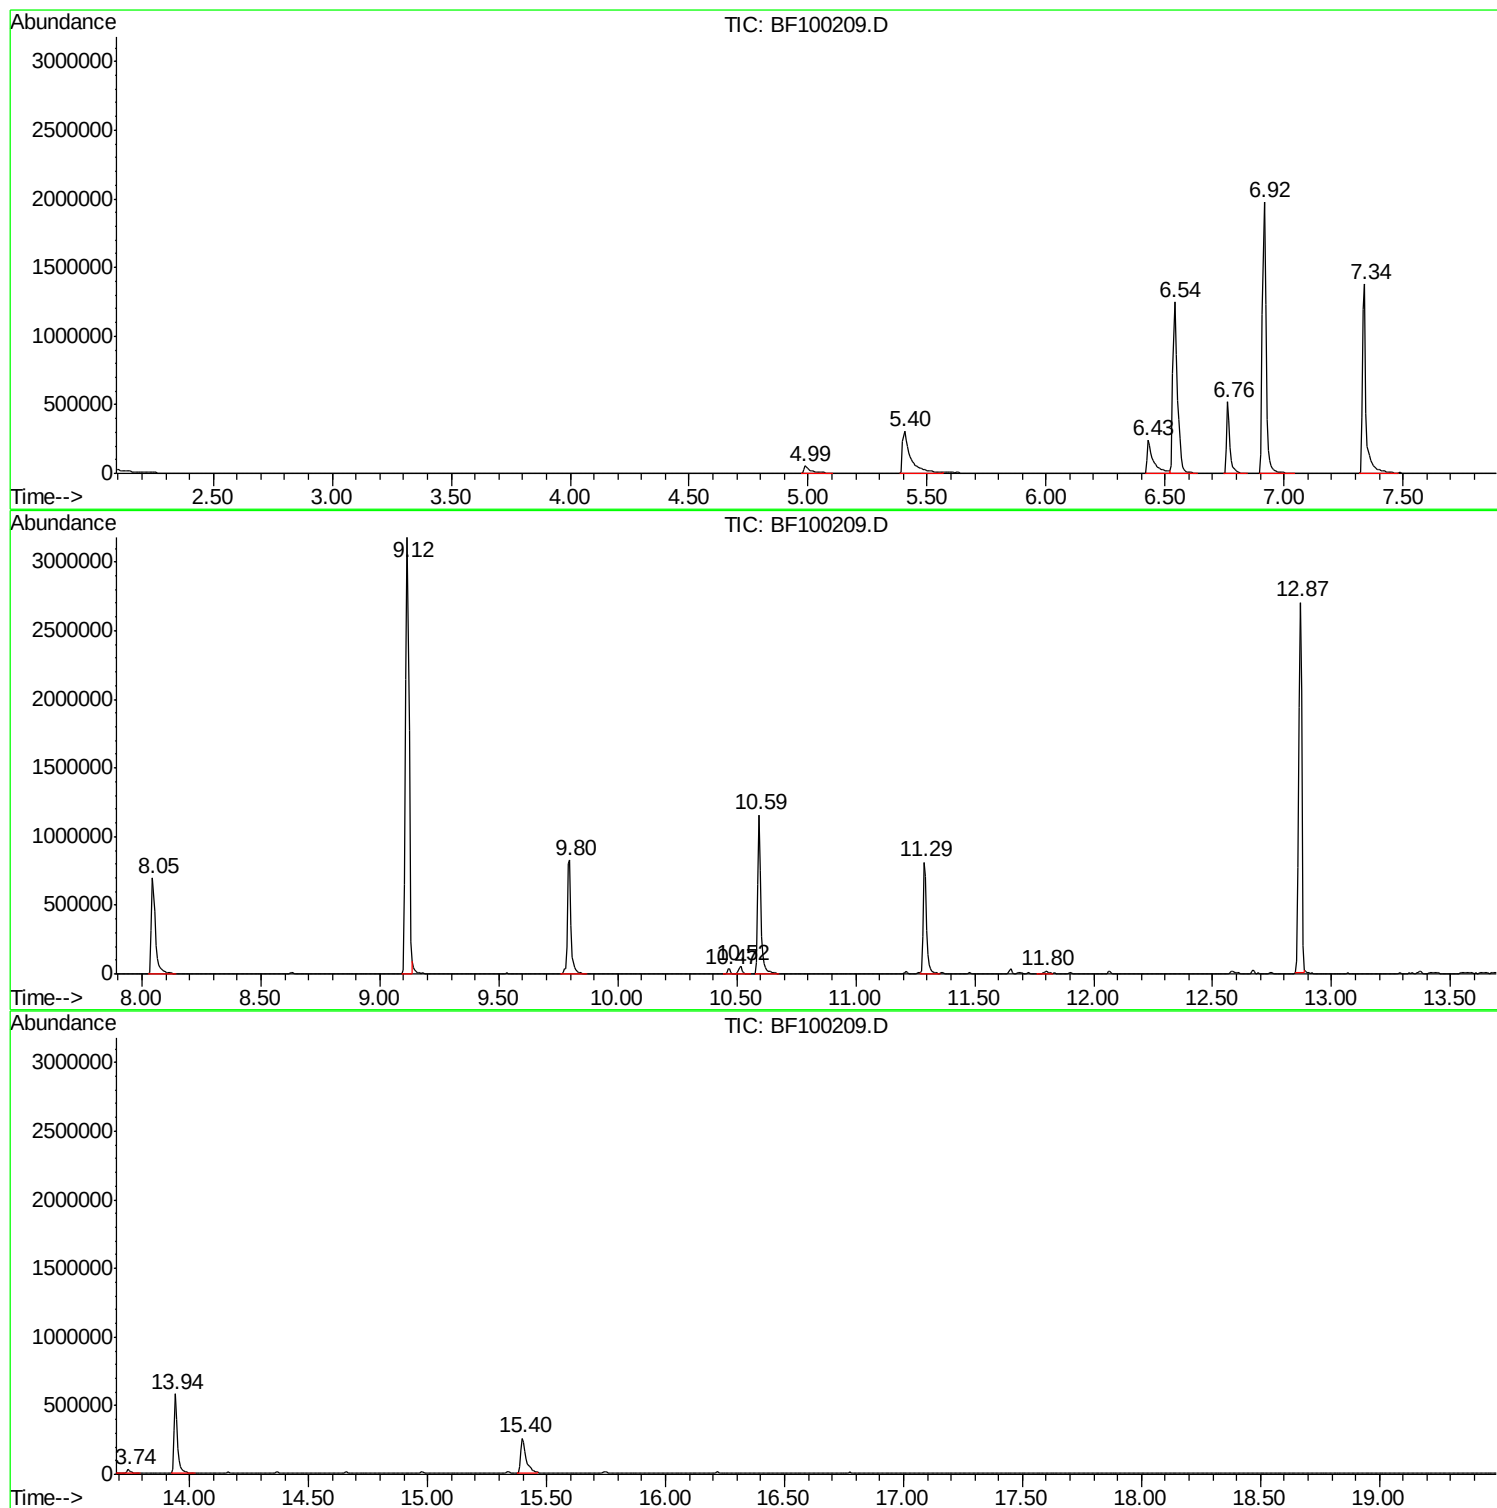

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100209.D
Acq_On : 5-Nov-2017 5:322
Operator : SJ/JUU
Sample : I6327-088
Misc :
ALS_Vial : 38 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-JETT-F-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
