

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100211.D
 Acq On : 5 Nov 2017 6:25
 Operator : SJ/JU
 Sample : I6327-10
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-SIDI-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	491	493	511	rBV	46675	105799	3.95%	0.672%
2	5.404	561	564	585	rBV	277054	612542	22.87%	3.893%
3	6.428	736	738	754	rBV	216046	419930	15.68%	2.669%
4	6.540	754	757	778	rVB	1112693	1378093	51.46%	8.759%
5	6.763	792	795	810	rVB	459719	454467	16.97%	2.889%
6	6.916	818	821	845	rBV	1840138	1785543	66.67%	11.349%
7	7.334	889	892	917	rBV	1145550	1367283	51.05%	8.691%
8	8.045	1010	1013	1032	rBV	609692	645640	24.11%	4.104%
9	9.116	1191	1195	1198	rBV	2956607	2678087	100.00%	17.022%
10	9.798	1302	1311	1322	rBV	762074	794721	29.67%	5.051%
11	10.463	1421	1424	1430	rBV	45446	38879	1.45%	0.247%
12	10.516	1430	1433	1440	rVB	41587	37157	1.39%	0.236%
13	10.592	1443	1446	1459	rBV	1065155	1063677	39.72%	6.761%
14	11.286	1561	1564	1575	rVB	748266	772900	28.86%	4.913%
15	11.651	1622	1626	1629	rBV	39990	33335	1.24%	0.212%
16	12.869	1829	1833	1836	rBV	2594068	2572528	96.06%	16.351%
17	13.739	1978	1981	1987	rBV3	23817	30155	1.13%	0.192%
18	13.939	2012	2015	2030	rVB	493063	558020	20.84%	3.547%
19	15.398	2259	2263	2277	rBV2	225148	384253	14.35%	2.442%


Sum of corrected areas: 15733009

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100211.D
Acq On : 5 Nov 2017 6:25
Operator : SJ/JU
Sample : I6327-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-D-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

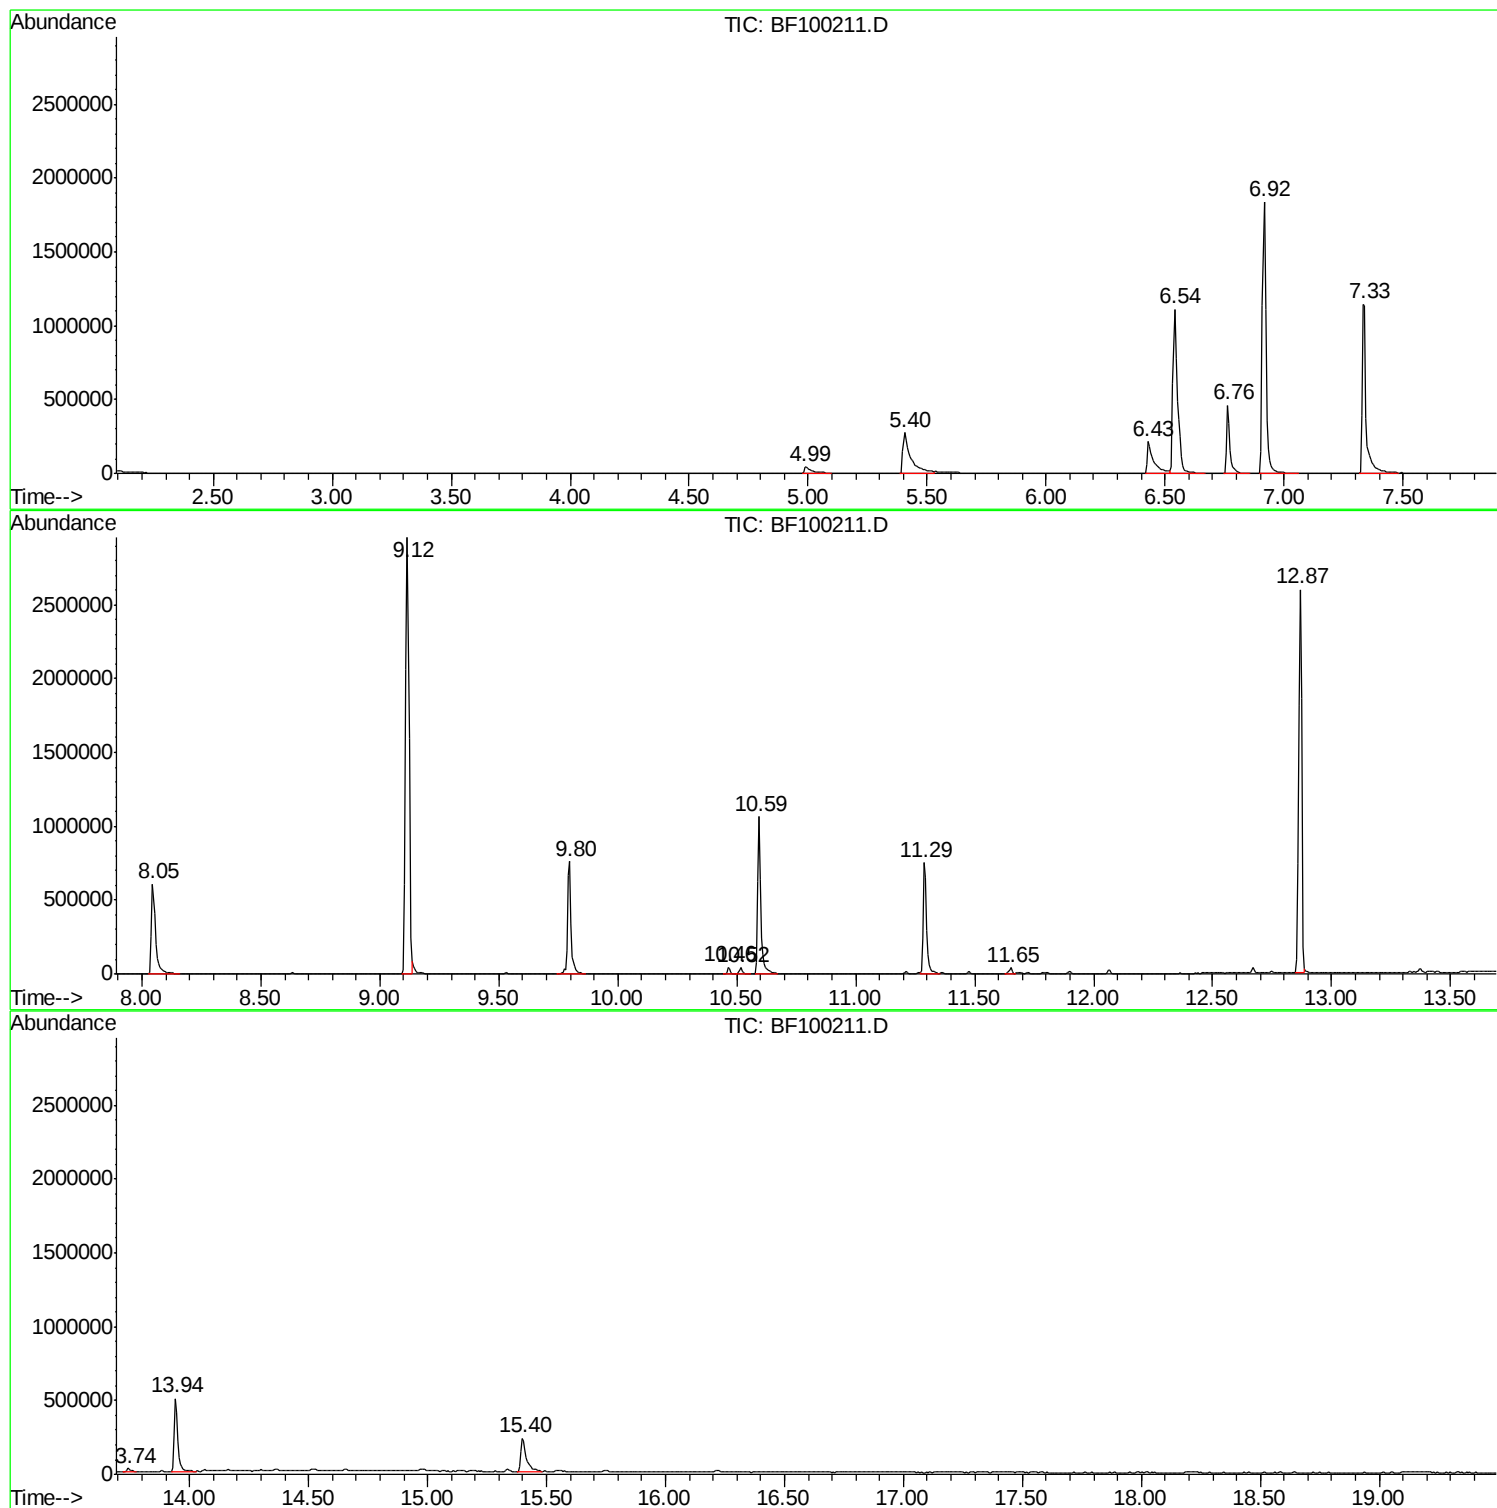

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100211.D
Acq_On : 5-Nov-2017 6:255
Operator : SJ/JUU
Sample : I6327-100
Misc :
ALS_Vial : 40 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-D-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
