

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100212.D
 Acq On : 5 Nov 2017 6:52
 Operator : SJ/JU
 Sample : I6327-11
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-SIDI-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	491	494	515	rBV	54023	117403	4.23%	0.696%
2	5.404	561	564	590	rBV	341189	749004	27.01%	4.440%
3	6.428	735	738	754	rBV	264518	532552	19.21%	3.157%
4	6.539	754	757	782	rVB	1279053	1509330	54.44%	8.947%
5	6.763	792	795	811	rVB	515228	517152	18.65%	3.066%
6	6.916	818	821	848	rBB	1931058	1885075	67.99%	11.175%
7	7.339	889	893	917	rBV	1280091	1443390	52.06%	8.556%
8	8.045	1010	1013	1037	rBV	663057	722010	26.04%	4.280%
9	9.116	1191	1195	1198	rBV	2988642	2772669	100.00%	16.436%
10	9.798	1305	1311	1323	rVB	881911	907056	32.71%	5.377%
11	10.463	1421	1424	1430	rVB	44481	40883	1.47%	0.242%
12	10.516	1430	1433	1439	rBB	34907	29111	1.05%	0.173%
13	10.592	1443	1446	1460	rBV	1017143	1067738	38.51%	6.330%
14	11.286	1561	1564	1576	rVB	774539	815876	29.43%	4.837%
15	12.668	1796	1799	1802	rBV	115715	86988	3.14%	0.516%
16	12.868	1829	1833	1836	rBV	2620942	2586743	93.29%	15.334%
17	13.368	1915	1918	1922	rVB	67938	60735	2.19%	0.360%
18	13.739	1978	1981	1992	rVB	28594	34186	1.23%	0.203%
19	13.939	2012	2015	2027	rBV	537407	584431	21.08%	3.465%
20	15.398	2259	2263	2282	rBV	255710	406779	14.67%	2.411%


Sum of corrected areas: 16869111

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100212.D
Acq On : 5 Nov 2017 6:52
Operator : SJ/JU
Sample : I6327-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

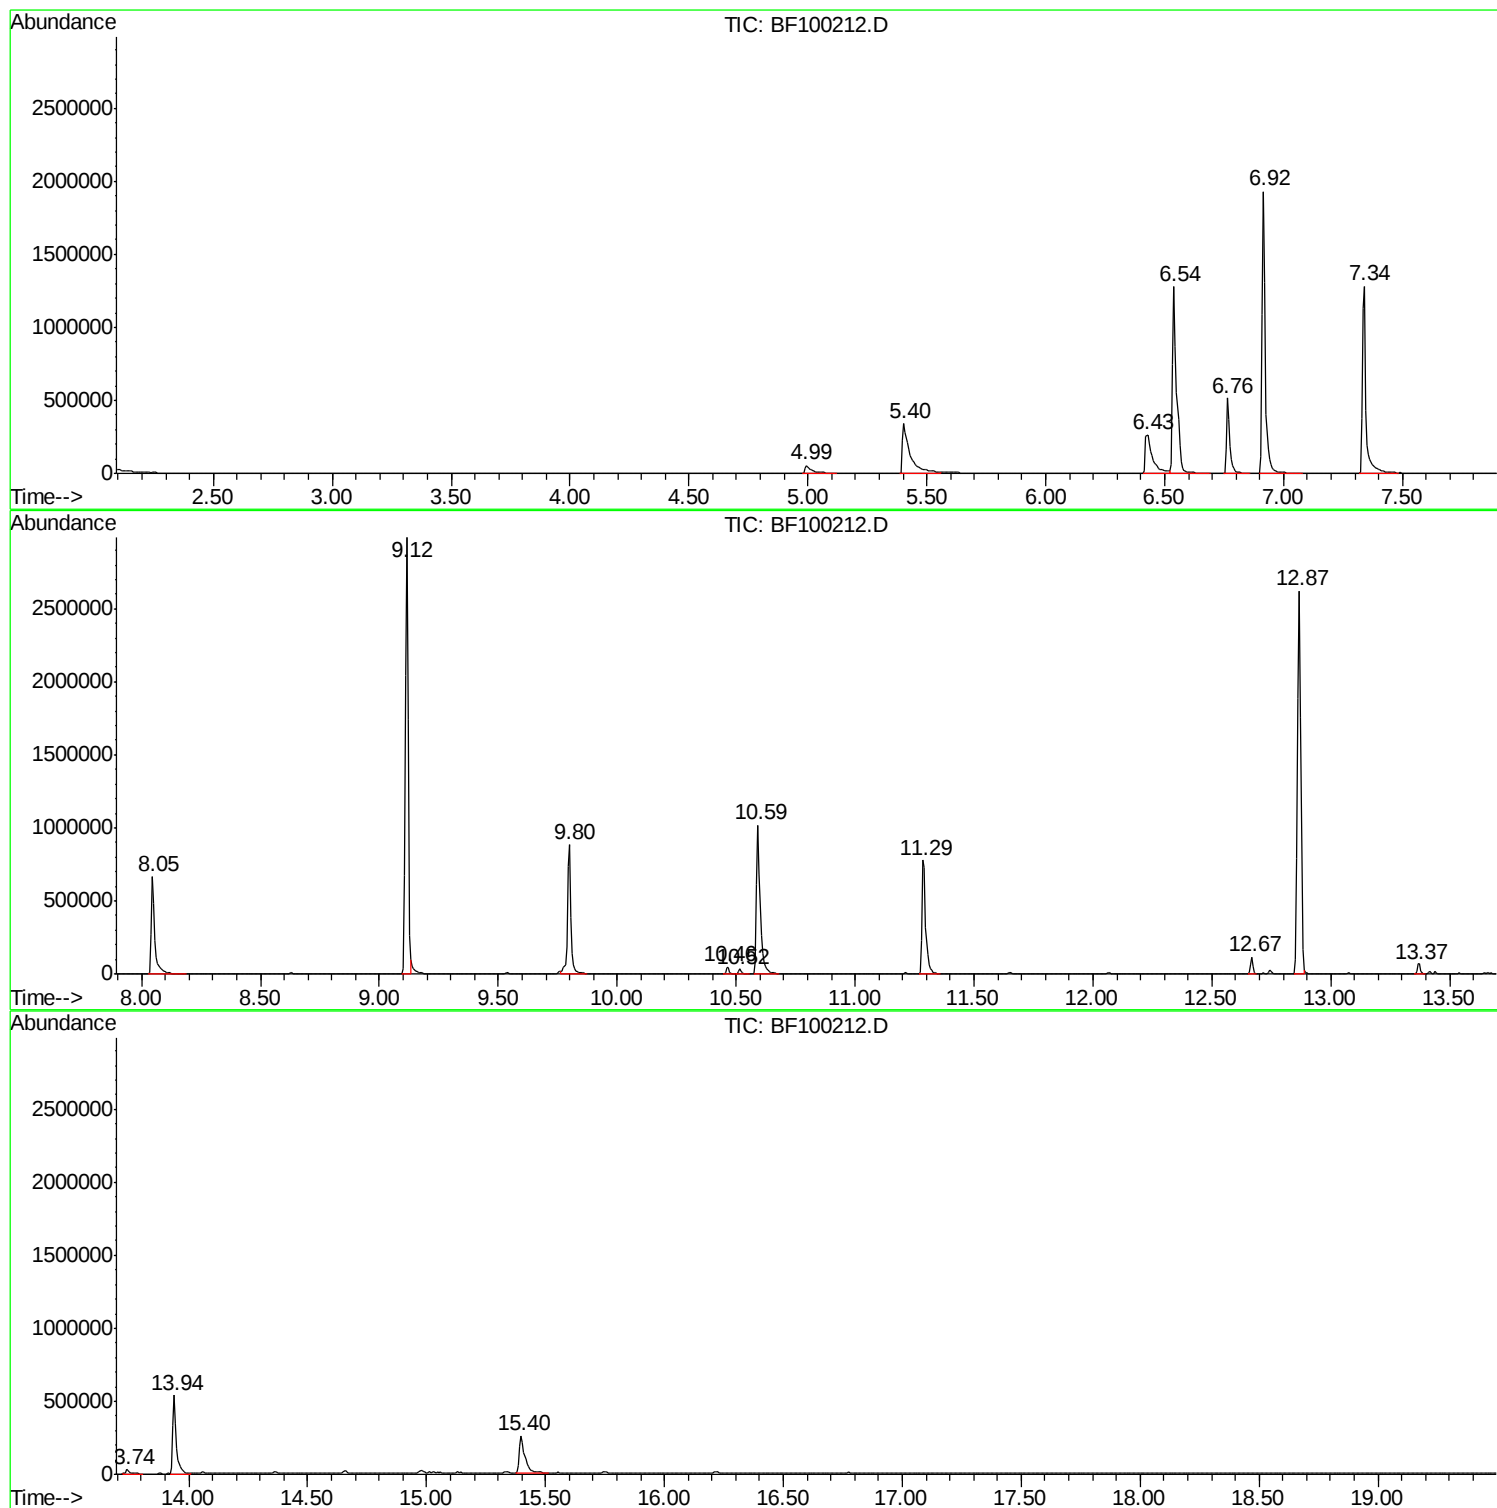

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100212.D
Acq_On : 5-Nov-2017 6:522
Operator : SJ/JUU
Sample : I6327-111
Misc :
ALS_Vial : 41 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-U-B

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
