

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
 Data File : BF100213.D
 Acq On : 5 Nov 2017 7:18
 Operator : SJ/JU
 Sample : I6327-12
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110217-SIDI-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	491	494	516	rBV	45507	102801	3.57%	0.603%
2	5.404	561	564	586	rBV	315790	711526	24.69%	4.172%
3	6.428	735	738	754	rBV	238498	464631	16.13%	2.724%
4	6.539	754	757	771	rVB	1266631	1497266	51.97%	8.778%
5	6.763	793	795	812	rVB	494055	493077	17.11%	2.891%
6	6.916	818	821	847	rBV	2016627	1913915	66.43%	11.221%
7	7.339	889	893	917	rBV	1415060	1504930	52.23%	8.823%
8	8.045	1010	1013	1028	rBV	655042	681694	23.66%	3.997%
9	9.116	1191	1195	1198	rBV	3066557	2881290	100.00%	16.893%
10	9.798	1305	1311	1327	rBB	822618	834967	28.98%	4.895%
11	10.469	1422	1425	1431	rBB	33725	29900	1.04%	0.175%
12	10.592	1443	1446	1460	rBV	1121138	1158880	40.22%	6.795%
13	11.286	1561	1564	1576	rVB	768702	812273	28.19%	4.762%
14	12.668	1796	1799	1802	rBV	80120	59368	2.06%	0.348%
15	12.868	1828	1833	1836	rBV	2683747	2780001	96.48%	16.299%
16	13.374	1916	1919	1922	rBV	50917	42143	1.46%	0.247%
17	13.739	1978	1981	1996	rVB2	40347	57307	1.99%	0.336%
18	13.939	2012	2015	2027	rBV	516620	572957	19.89%	3.359%
19	15.339	2249	2253	2257	rBV	25064	30454	1.06%	0.179%
20	15.398	2259	2263	2279	rBV2	232942	394541	13.69%	2.313%
21	16.215	2398	2402	2410	rVB2	17408	32154	1.12%	0.189%


Sum of corrected areas: 17056075

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110417\
Data File : BF100213.D
Acq On : 5 Nov 2017 7:18
Operator : SJ/JU
Sample : I6327-12
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-U-S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

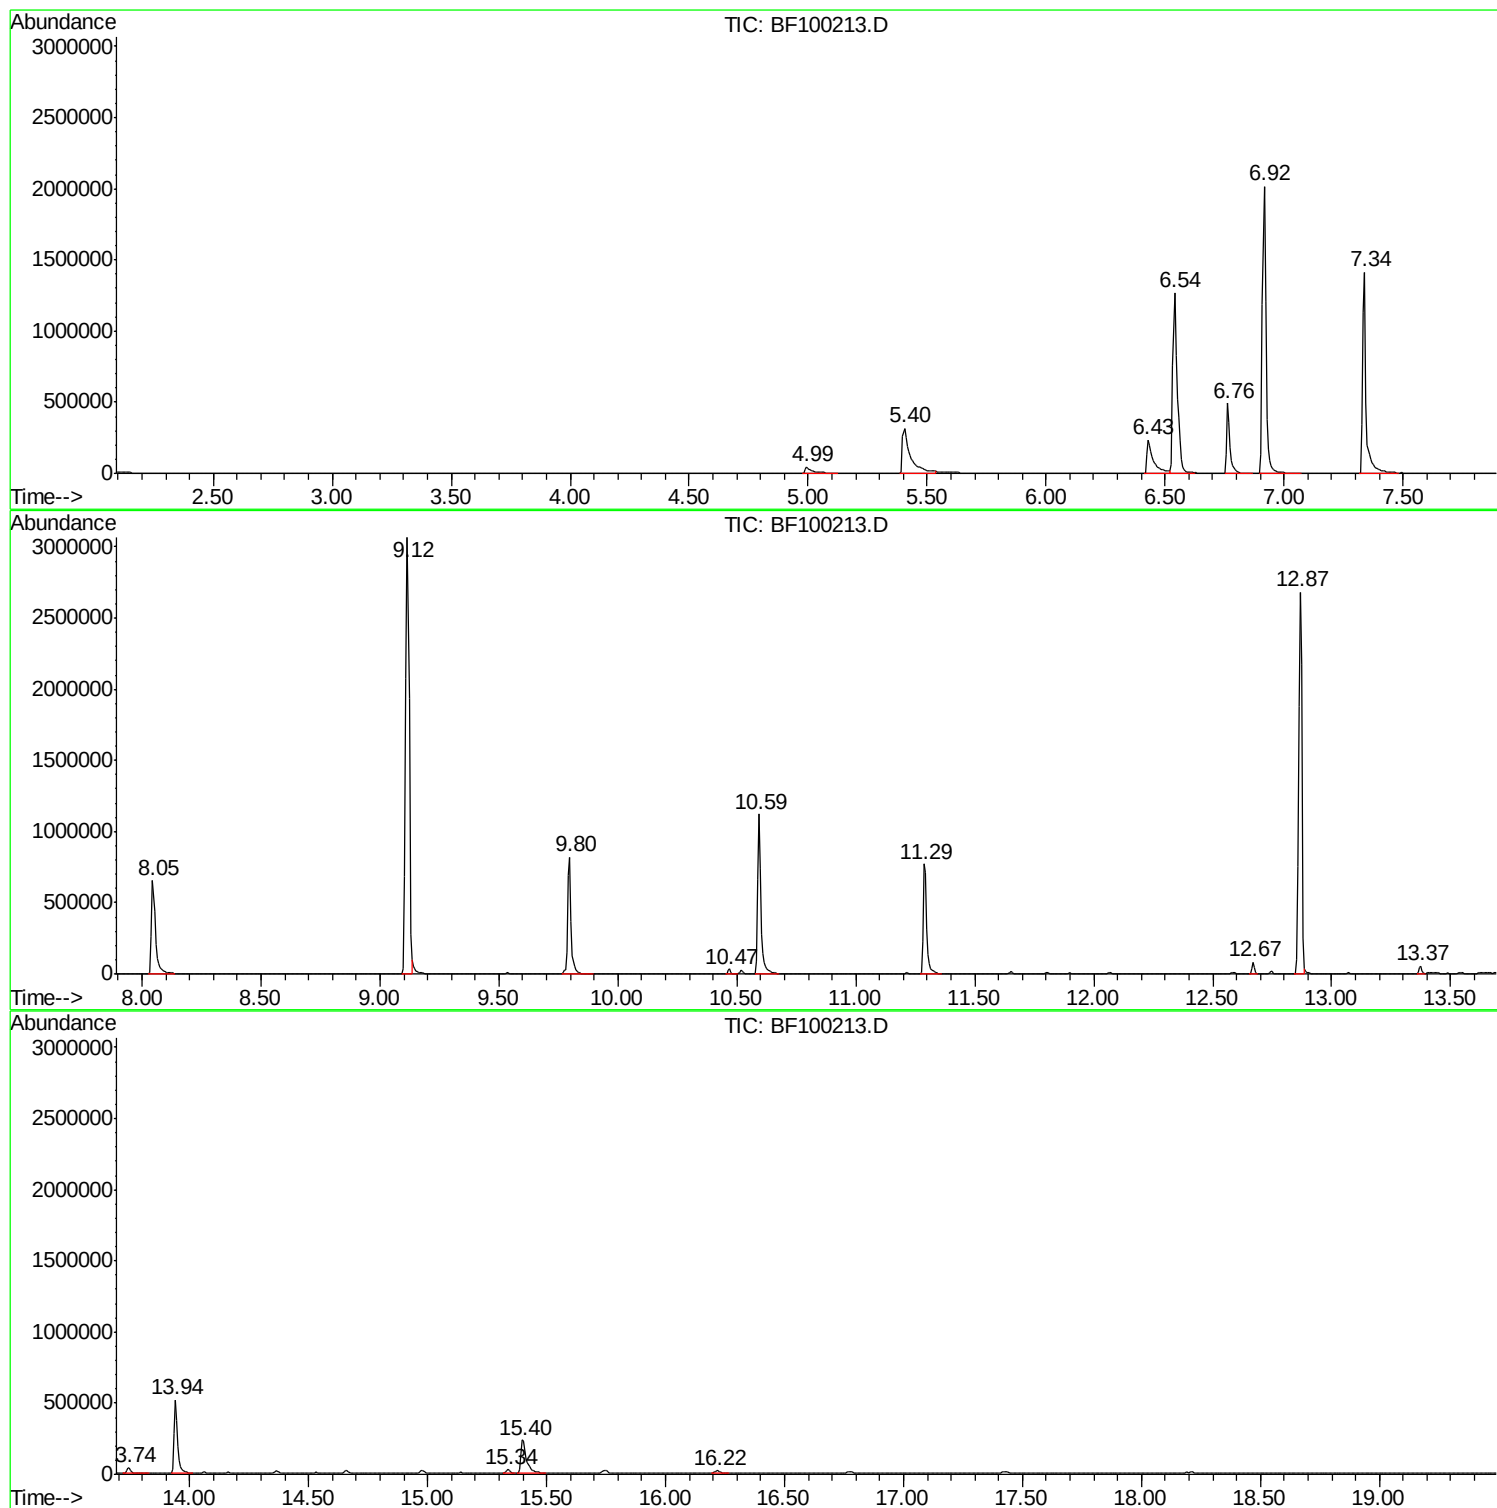

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110417\
Data_File : BF100213.D
Acq_On : 5-Nov-2017 7:188
Operator : SJ/JUU
Sample : I6327-122
Misc :
ALS_Vial : 42 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
110217-SIDI-F-U-S

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
