

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110420\
 Data File : BF122276.D
 Acq On : 4 Nov 2020 21:51
 Operator : JU/CG
 Sample : L4613-03 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 282

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.252	365	368	381	rBV	39319	97584	16.65%	2.221%
2	4.899	475	478	496	rBV	52469	118258	20.17%	2.691%
3	5.446	564	571	574	rBV3	5791	11580	1.98%	0.264%
4	6.440	736	740	749	rBV2	29233	91775	15.66%	2.088%
5	6.710	783	786	797	rBV	429712	471520	80.43%	10.730%
6	7.304	884	887	906	rBV	47281	117261	20.00%	2.668%
7	7.998	1001	1005	1024	rBV	430896	559349	95.41%	12.729%
8	8.581	1099	1104	1108	rBV	11866	13077	2.23%	0.298%
9	9.075	1184	1188	1196	rBV	148738	196739	33.56%	4.477%
10	9.145	1196	1200	1203	rVB	18703	20815	3.55%	0.474%
11	9.463	1249	1254	1256	rBV4	11207	16430	2.80%	0.374%
12	9.486	1256	1258	1261	rVB2	10555	11279	1.92%	0.257%
13	9.675	1287	1290	1293	rBV	22693	24751	4.22%	0.563%
14	9.745	1299	1302	1317	rBV	491167	586233	100.00%	13.341%
15	9.992	1341	1344	1347	rBV3	8905	10474	1.79%	0.238%
16	10.169	1371	1374	1378	rBV	30438	27355	4.67%	0.623%
17	10.386	1406	1411	1414	rBV2	17355	18981	3.24%	0.432%
18	10.645	1451	1455	1463	rVB2	36565	56298	9.60%	1.281%
19	11.086	1527	1530	1533	rBV	24884	24981	4.26%	0.568%
20	11.116	1533	1535	1542	rVB3	22555	22630	3.86%	0.515%
21	11.239	1552	1556	1570	rBV	488777	573538	97.83%	13.052%
22	11.516	1599	1603	1606	rBV	25767	23311	3.98%	0.530%
23	11.922	1669	1672	1676	rBV	23338	21701	3.70%	0.494%
24	12.310	1733	1738	1742	rBV2	18895	23550	4.02%	0.536%
25	12.463	1761	1764	1767	rBV	11665	13430	2.29%	0.306%
26	12.692	1798	1803	1808	rBV2	22007	37649	6.42%	0.857%
27	12.816	1821	1824	1834	rBV	255299	253159	43.18%	5.761%
28	13.886	2003	2006	2013	rBV	504625	566686	96.67%	12.896%
29	15.333	2248	2252	2261	rVB	253046	383936	65.49%	8.737%


Sum of corrected areas: 4394330

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110420\
Data File : BF122276.D
Acq On : 4 Nov 2020 21:51
Operator : JU/CG
Sample : L4613-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
282

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

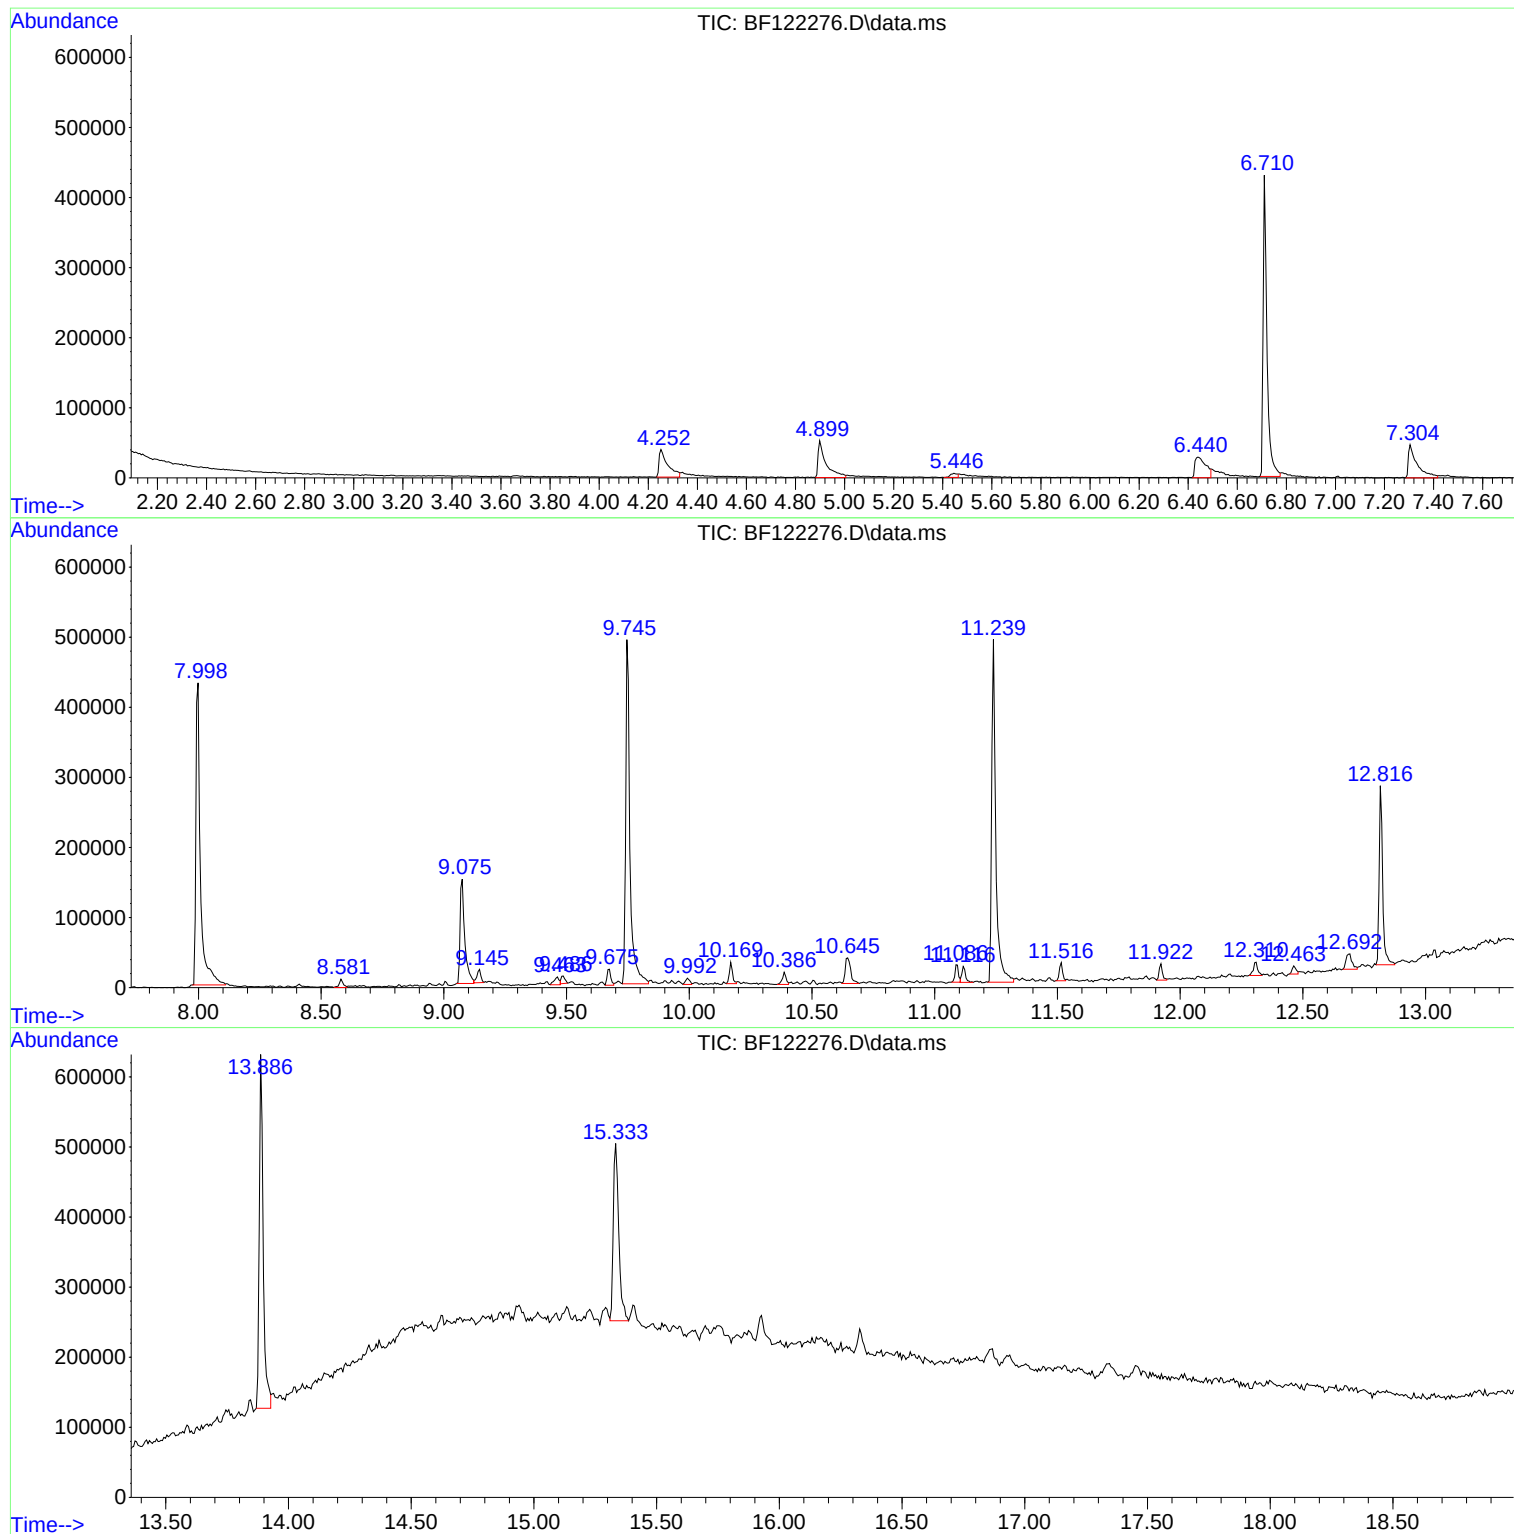

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110420\
Data File : BF122276.D
Acq On : 4 Nov 2020 21:51
Operator : JU/CG
Sample : L4613-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
282

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110420\
Data File : BF122276.D
Acq On : 4 Nov 2020 21:51
Operator : JU/CG
Sample : L4613-03 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
282

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
