
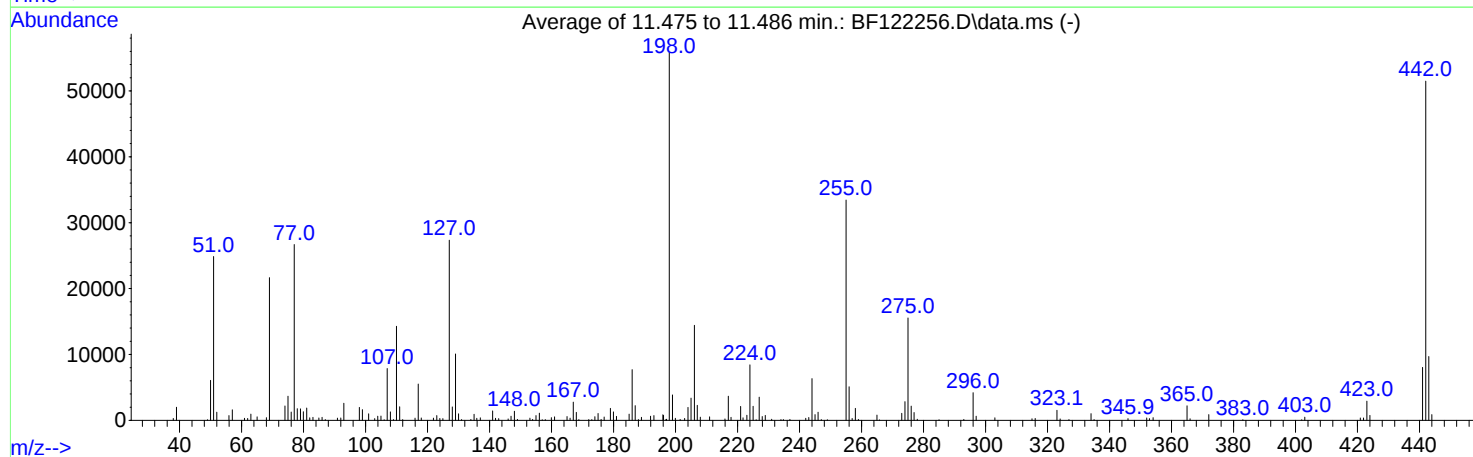


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110420\
 Data File : BF122256.D
 Acq On : 4 Nov 2020 11:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 10:16:54 2020

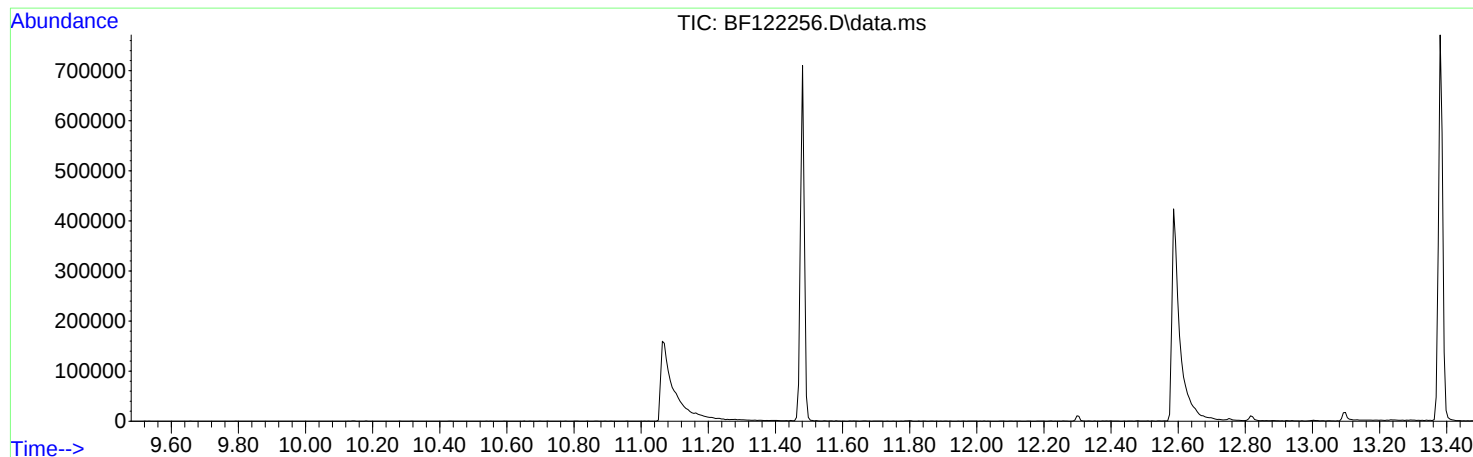

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	24855	PASS
68	69	0.00	2	1.9	418	PASS
69	198	0.00	100	38.8	21652	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	27340	PASS
197	198	0.00	2	0.3	183	PASS
198	198	100	100	100.0	55827	PASS
199	198	5	9	6.9	3850	PASS
275	198	10	60	27.8	15544	PASS
365	198	1	100	4.0	2209	PASS
441	198	0.01	100	14.4	8044	PASS
442	198	50	100	92.2	51475	PASS
443	442	15	24	18.8	9682	PASS