
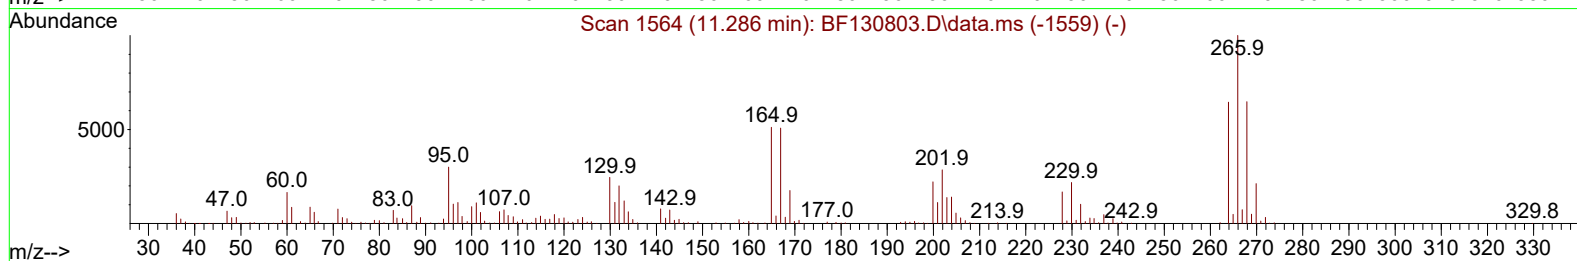
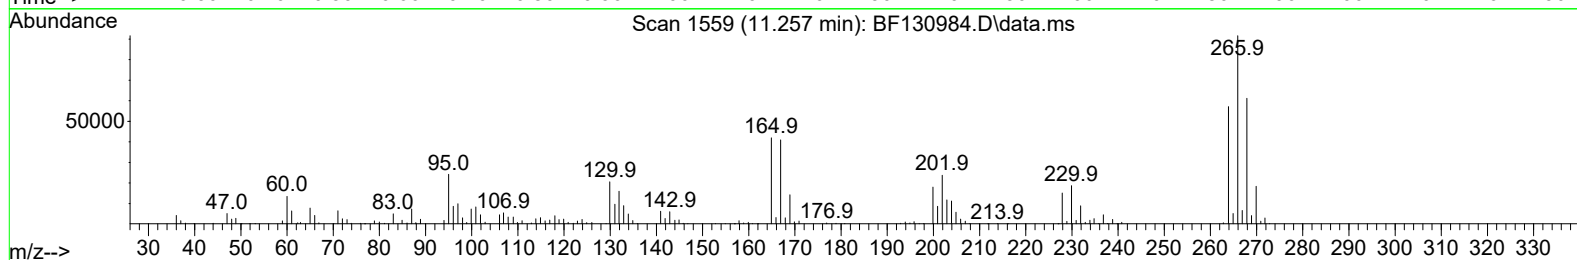


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130984.D
Acq On : 04 Nov 2022 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 04:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

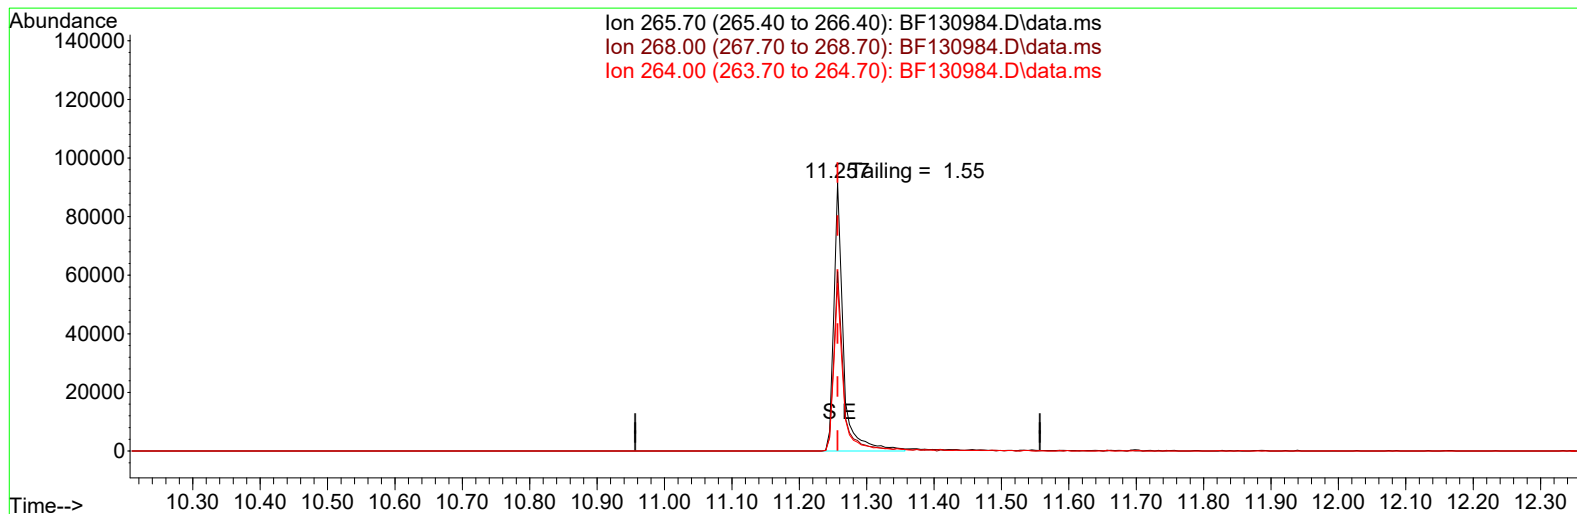

TIC: BF130984.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 19243.67 ng

response 90159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.79
264.00	64.50	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130984.D
Acq On : 04 Nov 2022 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 04:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

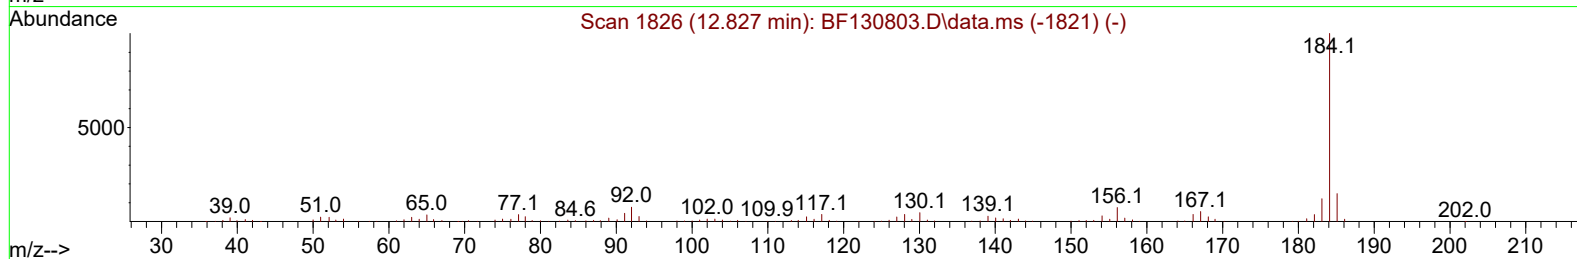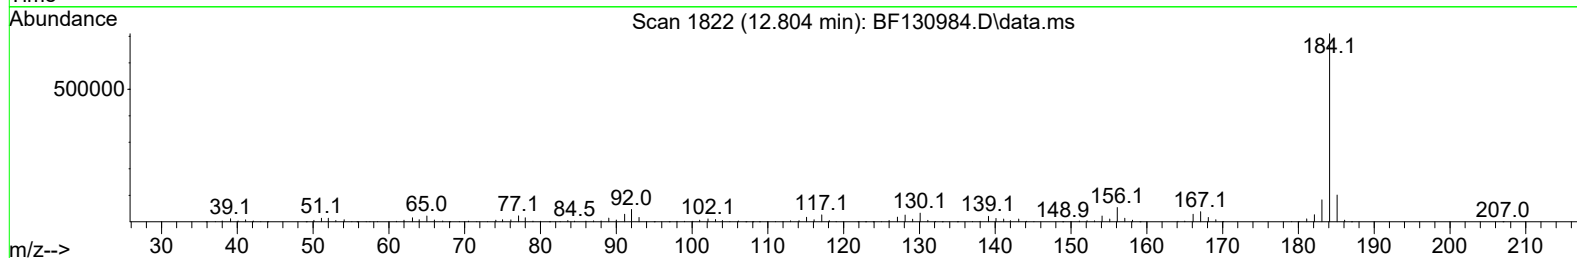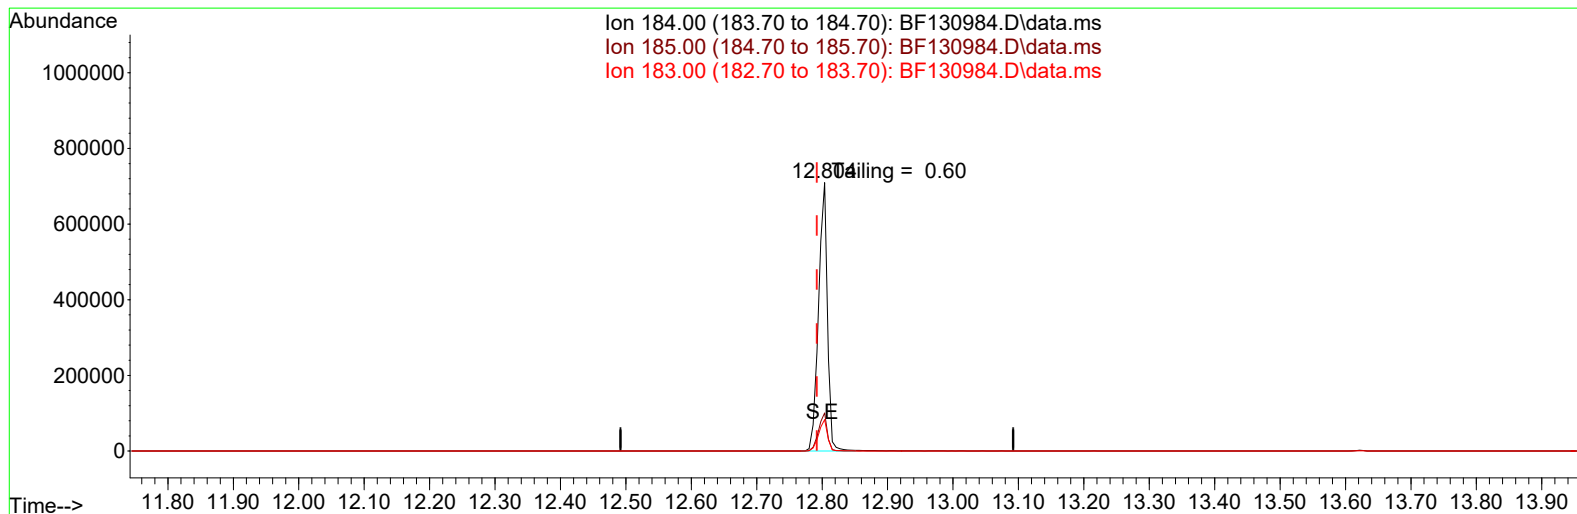

TIC: BF130984.D\data.ms

(77) Benzidine**12.804min (+ 0.012) 479347.71 ng****response 674896**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.19
183.00	12.10	11.70
0.00	0.00	0.00