

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF130996.D
 Acq On : 04 Nov 2022 18:04
 Operator : CG\JU
 Sample : N5435-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PTS-CON-1103

Quant Time: Nov 05 00:38:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.910	152	66943	20.000	ng	0.00
21) Naphthalene-d8	8.198	136	210312	20.000	ng	# 0.00
39) Acenaphthene-d10	9.957	164	112217	20.000	ng	0.00
64) Phenanthrene-d10	11.451	188	192205	20.000	ng	0.00
76) Chrysene-d12	14.098	240	144584	20.000	ng	0.00
86) Perylene-d12	15.604	264	124757	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	286111	74.094	ng	0.00
7) Phenol-d6	6.534	99	470383	93.739	ng	0.00
23) Nitrobenzene-d5	7.475	82	268202	76.897	ng	-0.01
42) 2,4,6-Tribromophenol	10.751	330	83038	87.904	ng	0.00
45) 2-Fluorobiphenyl	9.275	172	477613	64.348	ng	0.00
79) Terphenyl-d14	13.039	244	449650	56.989	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130996.D
Acq On : 04 Nov 2022 18:04
Operator : CG\JU
Sample : N5435-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PTS-CON-1103

Quant Time: Nov 05 00:38:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration




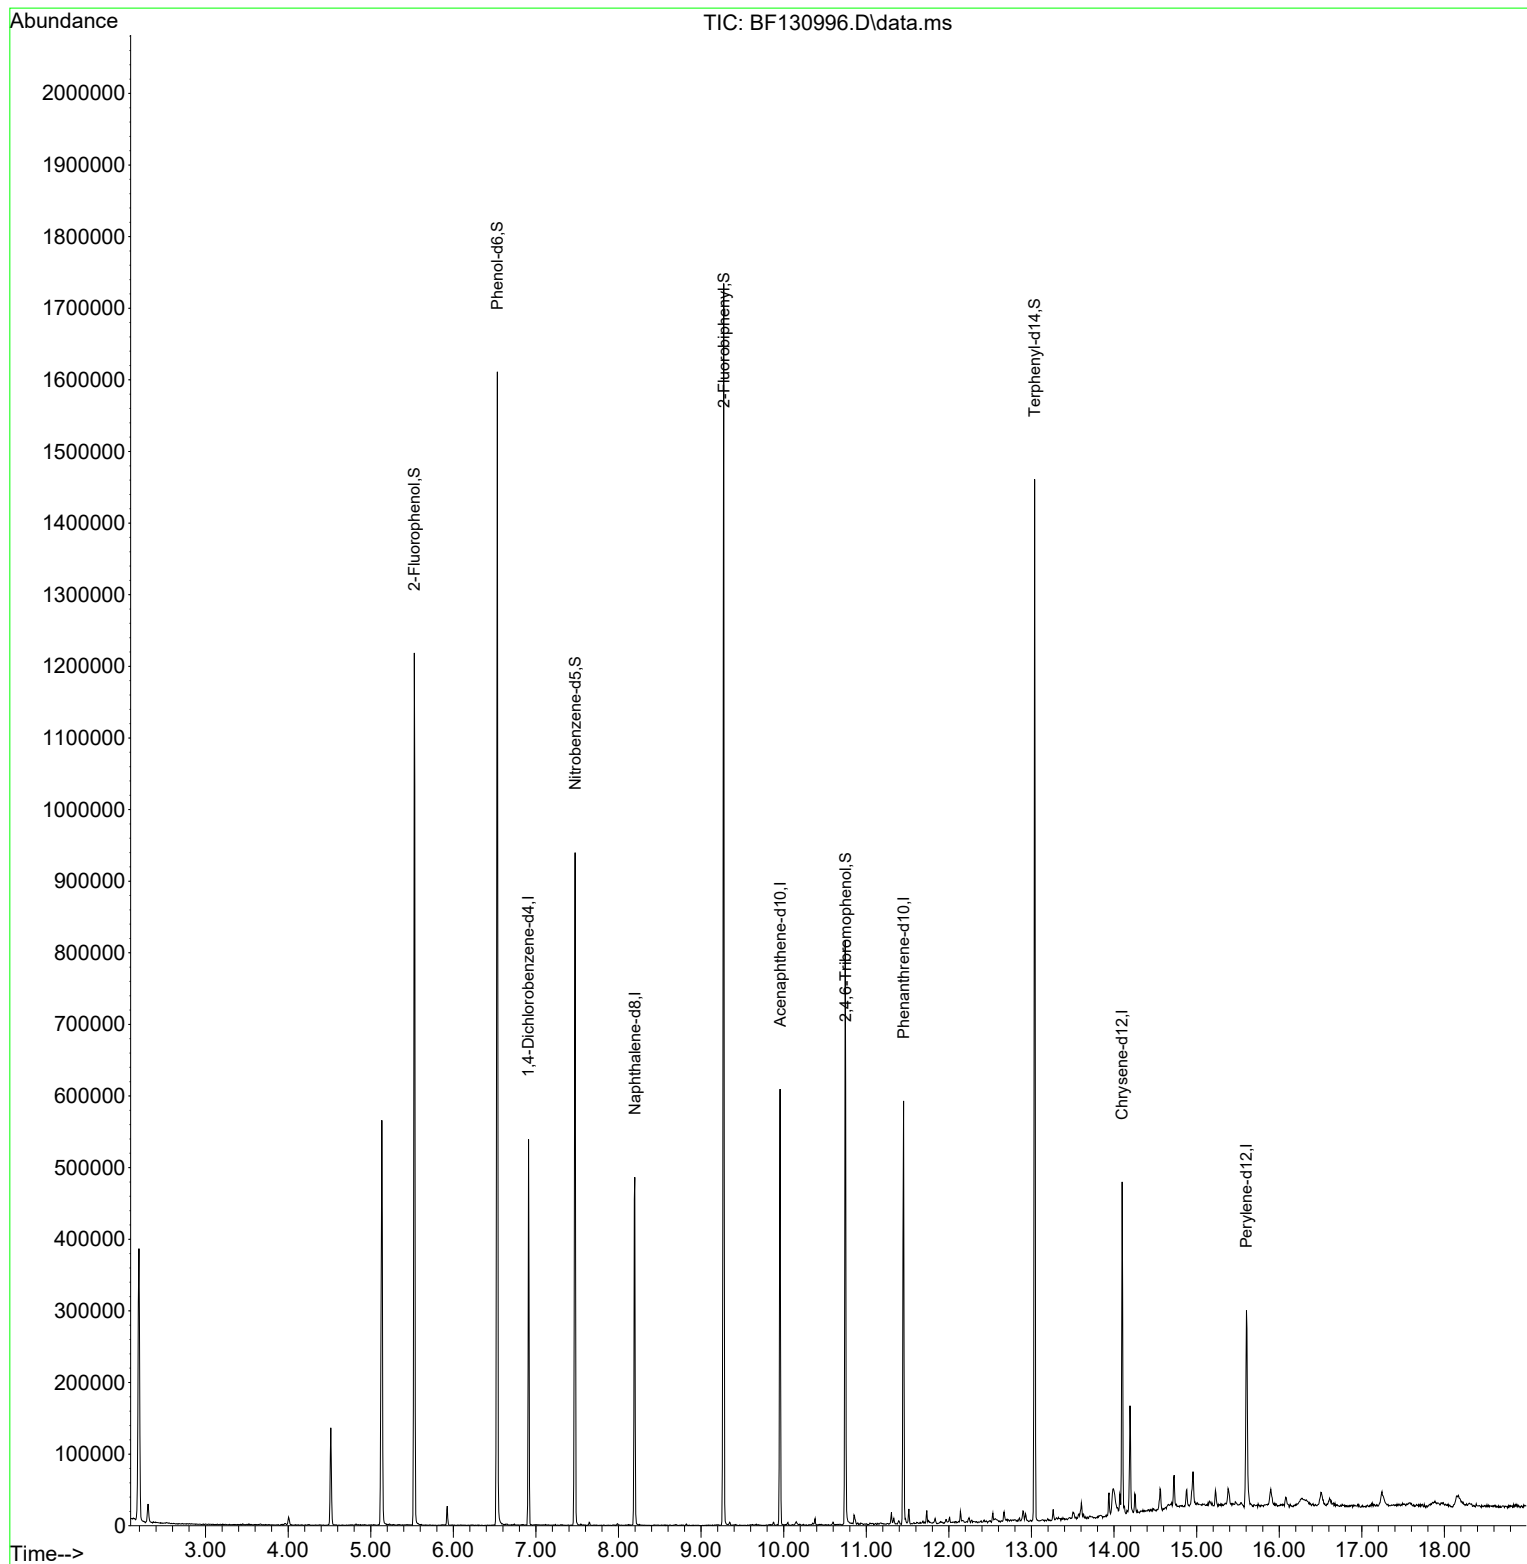




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.910 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04




Instrument :
BNA_F
ClientSampleId :
PTS-CON-1103

Tgt Ion:152 Resp: 66943
Ion Ratio Lower Upper
152 100
150 152.5 124.1 186.1
115 67.0 50.1 75.1

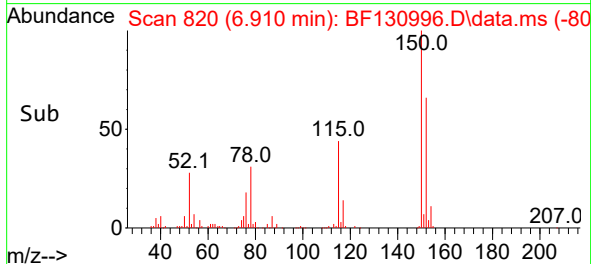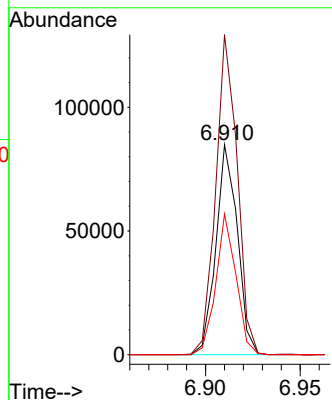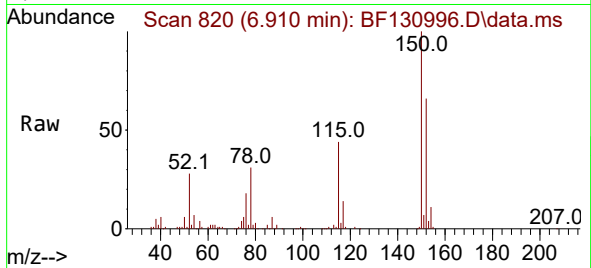

#5
2-Fluorophenol
Concen: 74.094 ng
RT: 5.528 min Scan# 585
Delta R.T. -0.000 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04

Tgt Ion:112 Resp: 286111
Ion Ratio Lower Upper
112 100
64 70.5 53.9 80.9
63 40.4 29.4 44.2


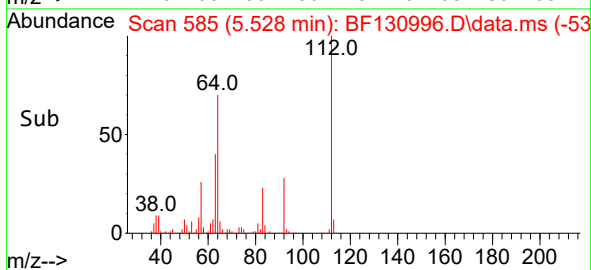
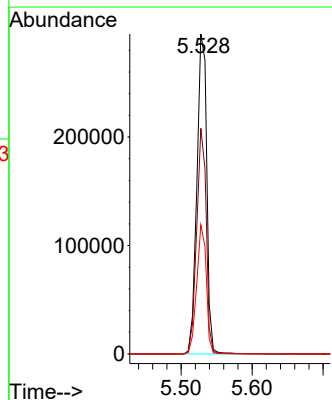
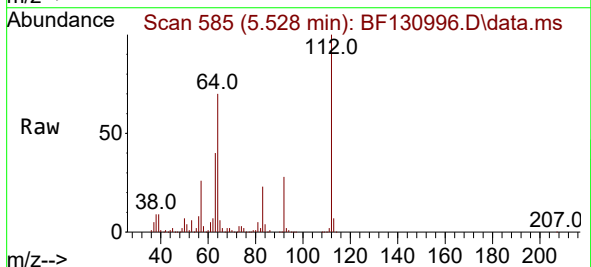




#7
Phenol-d6
Concen: 93.739 ng
RT: 6.534 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04




Instrument :
BNA_F
ClientSampleId :
PTS-CON-1103

Tgt Ion: 99 Resp: 470383
Ion Ratio Lower Upper
99 100
42 24.2 18.8 28.2
71 40.1 31.4 47.0

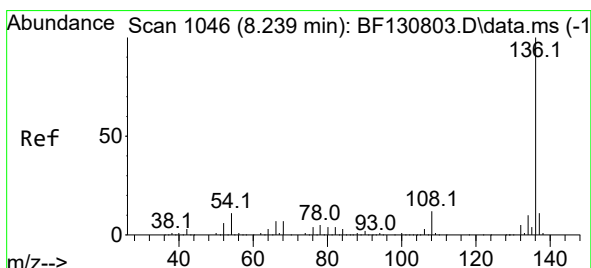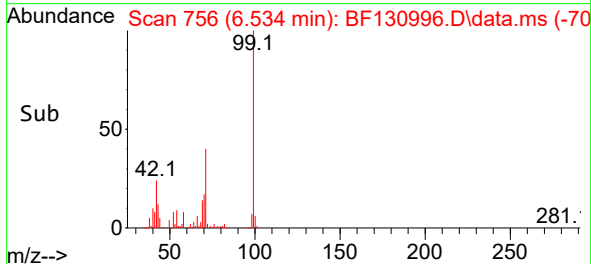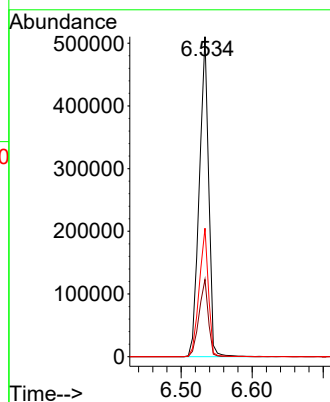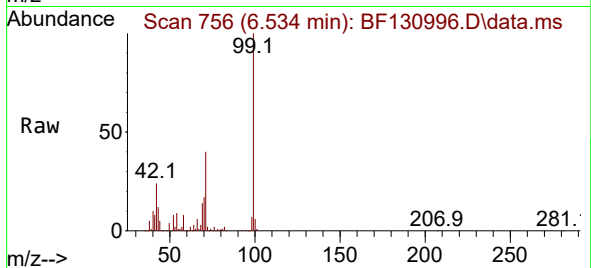

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.198 min Scan# 1039
Delta R.T. -0.006 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04

Tgt Ion: 136 Resp: 210312
Ion Ratio Lower Upper
136 100
137 10.6 9.2 13.8
54 8.9 8.8 13.2
68 4.8 5.2 7.8#

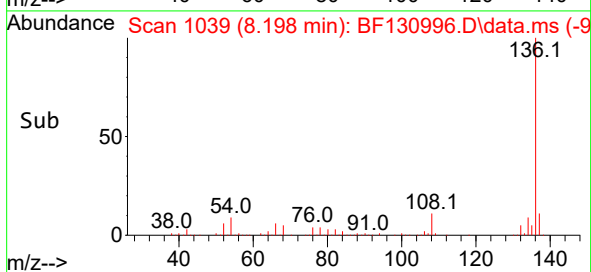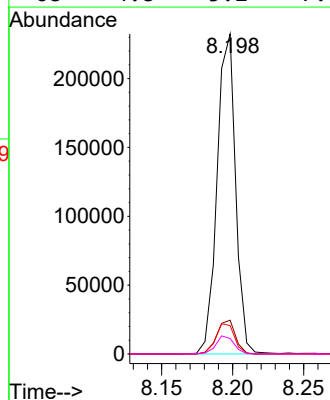



#23

Nitrobenzene-d5

Concen: 76.897 ng

RT: 7.475 min Scan# 91

Delta R.T. -0.012 min

Lab File: BF130996.D

Acq: 04 Nov 2022 18:04

Instrument :

BNA_F

ClientSampleId :

PTS-CON-1103





Tgt Ion: 82 Resp: 268202

Ion Ratio Lower Upper

82 100

128 39.1 31.2 46.8

54 60.4 48.0 72.0

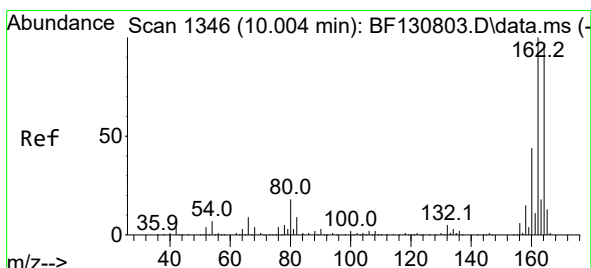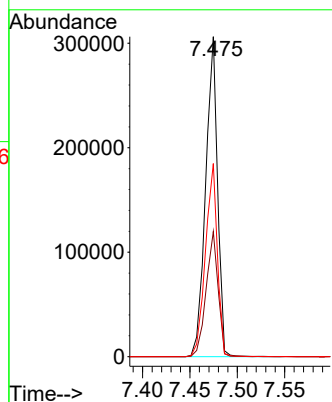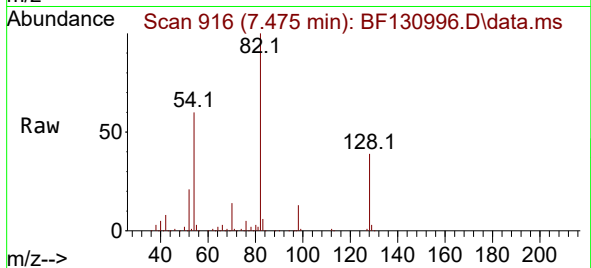

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.957 min Scan# 1338

Delta R.T. -0.006 min

Lab File: BF130996.D

Acq: 04 Nov 2022 18:04




Tgt Ion:164 Resp: 112217


Ion Ratio Lower Upper

164 100

162 101.6 82.2 123.2

160 45.6 36.6 54.8

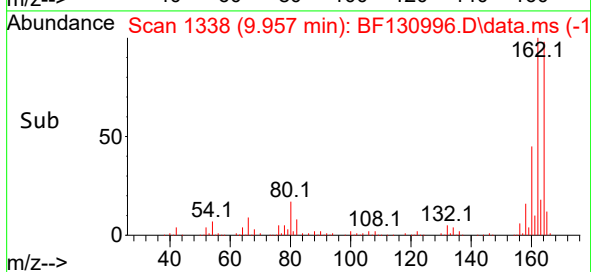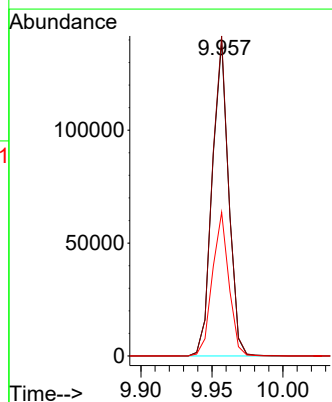



#42

2,4,6-Tribromophenol

Concen: 87.904 ng

RT: 10.751 min Scan# 1480

Delta R.T. -0.006 min

Lab File: BF130996.D


Acq: 04 Nov 2022 18:04

Instrument :

BNA_F

ClientSampleId :

PTS-CON-1103

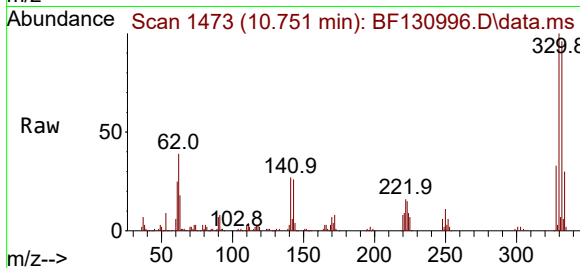




Tgt Ion:330 Resp: 83038

Ion Ratio Lower Upper

330 100

332 97.6 76.2 114.4

141 38.2 31.4 47.0

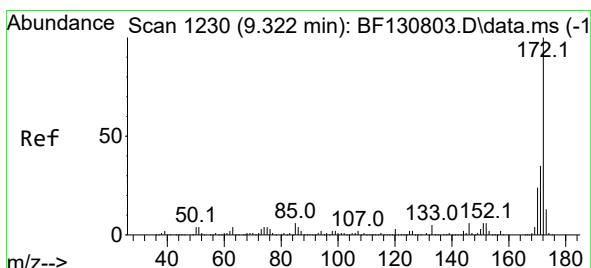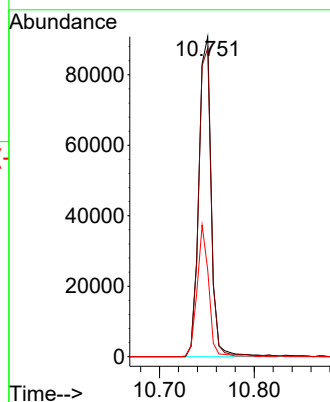

#45

2-Fluorobiphenyl

Concen: 64.348 ng

RT: 9.275 min Scan# 1222

Delta R.T. -0.006 min

Lab File: BF130996.D

Acq: 04 Nov 2022 18:04




Tgt Ion:172 Resp: 477613


Ion Ratio Lower Upper

172 100

171 35.2 28.1 42.1

170 23.3 19.0 28.4


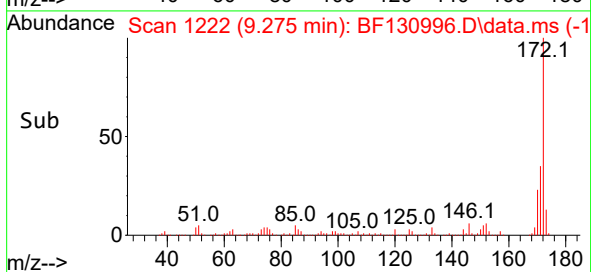

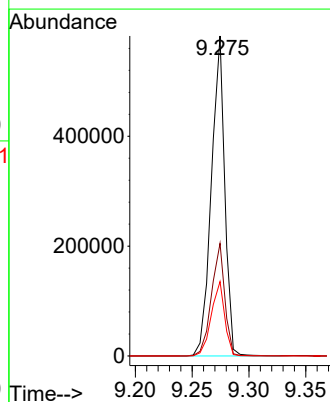




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04




Instrument :
BNA_F
ClientSampleId :
PTS-CON-1103


Tgt Ion:188 Resp: 192205
Ion Ratio Lower Upper
188 100
94 8.1 7.4 11.2
80 9.0 8.0 12.0

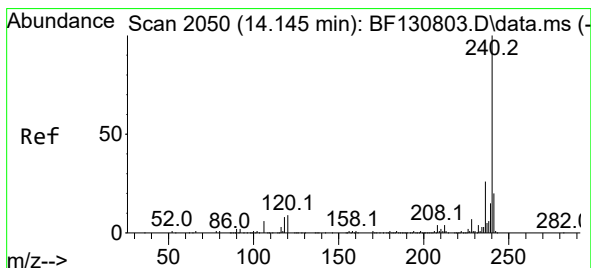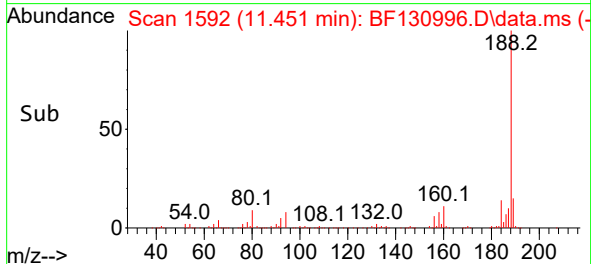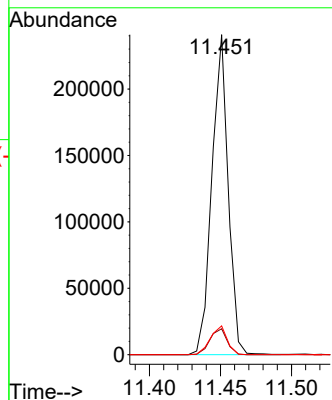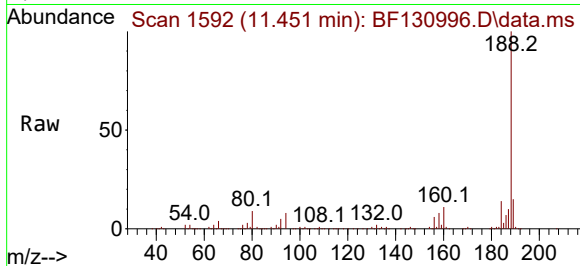

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.098 min Scan# 2042
Delta R.T. -0.006 min
Lab File: BF130996.D
Acq: 04 Nov 2022 18:04

Tgt Ion:240 Resp: 144584
Ion Ratio Lower Upper
240 100
120 10.4 7.0 10.4
236 25.1 20.5 30.7


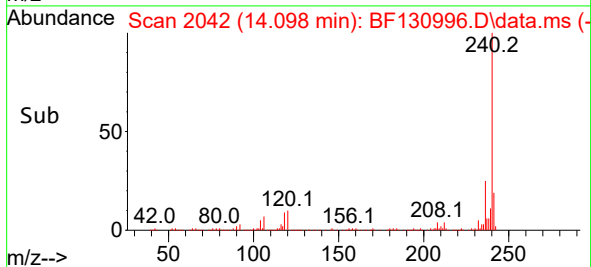
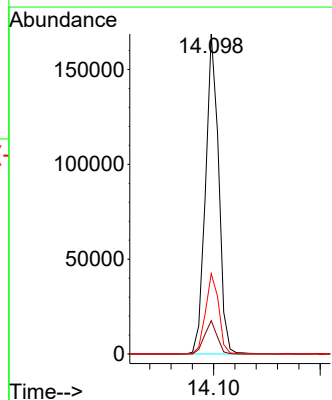
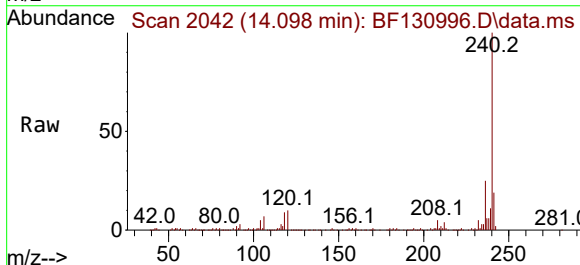




#79
 Terphenyl-d14
 Concen: 56.989 ng
 RT: 13.039 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF130996.D
 Acq: 04 Nov 2022 18:04

Instrument :
 BNA_F
 ClientSampleId :
 PTS-CON-1103

Tgt Ion:244 Resp: 449650
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.2
 122 10.1 7.9 11.9

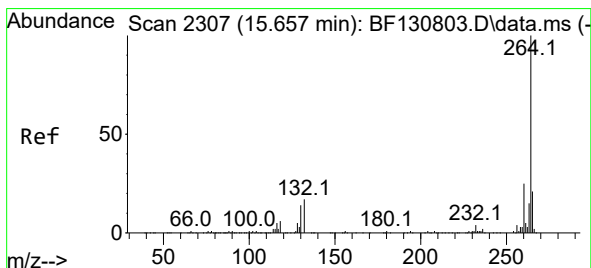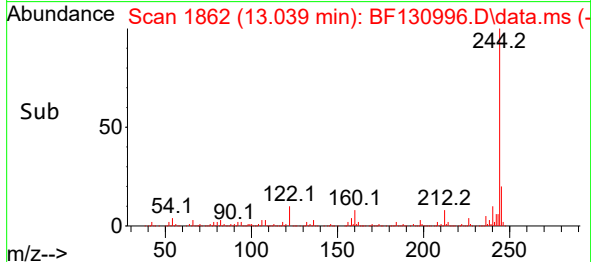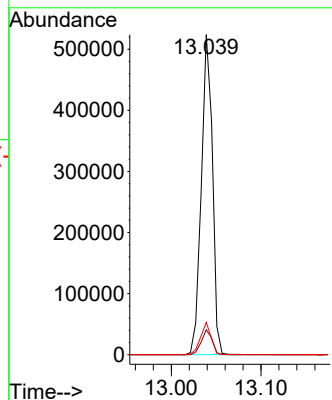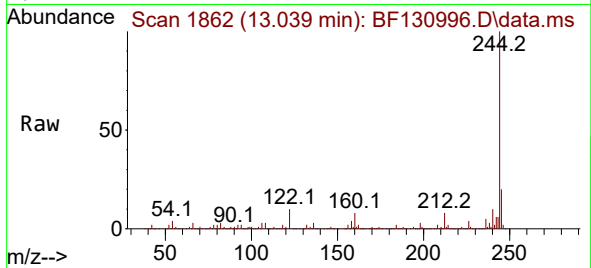

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.604 min Scan# 2298
 Delta R.T. -0.006 min
 Lab File: BF130996.D
 Acq: 04 Nov 2022 18:04

Tgt Ion:264 Resp: 124757
 Ion Ratio Lower Upper
 264 100
 260 23.0 19.9 29.9
 265 21.7 17.0 25.6

