

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF131007.D
 Acq On : 05 Nov 2022 00:10
 Operator : CG\JU
 Sample : N5318-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20221106-COMP-05

Quant Time: Nov 05 00:42:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.910	152	80388	20.000	ng	0.00
21) Naphthalene-d8	8.192	136	313849	20.000	ng	-0.01
39) Acenaphthene-d10	9.957	164	174469	20.000	ng	0.00
64) Phenanthrene-d10	11.451	188	335646	20.000	ng	0.00
76) Chrysene-d12	14.098	240	239489	20.000	ng	0.00
86) Perylene-d12	15.604	264	184926	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.534	112	509385	109.852	ng	0.00
7) Phenol-d6	6.534	99	653277	108.413	ng	0.00
23) Nitrobenzene-d5	7.475	82	435475	83.666	ng	-0.01
42) 2,4,6-Tribromophenol	10.751	330	185506	126.308	ng	0.00
45) 2-Fluorobiphenyl	9.275	172	743868	64.461	ng	0.00
79) Terphenyl-d14	13.039	244	835850	63.955	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF131007.D
Acq On : 05 Nov 2022 00:10
Operator : CG\JU
Sample : N5318-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20221106-COMP-05

Quant Time: Nov 05 00:42:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration




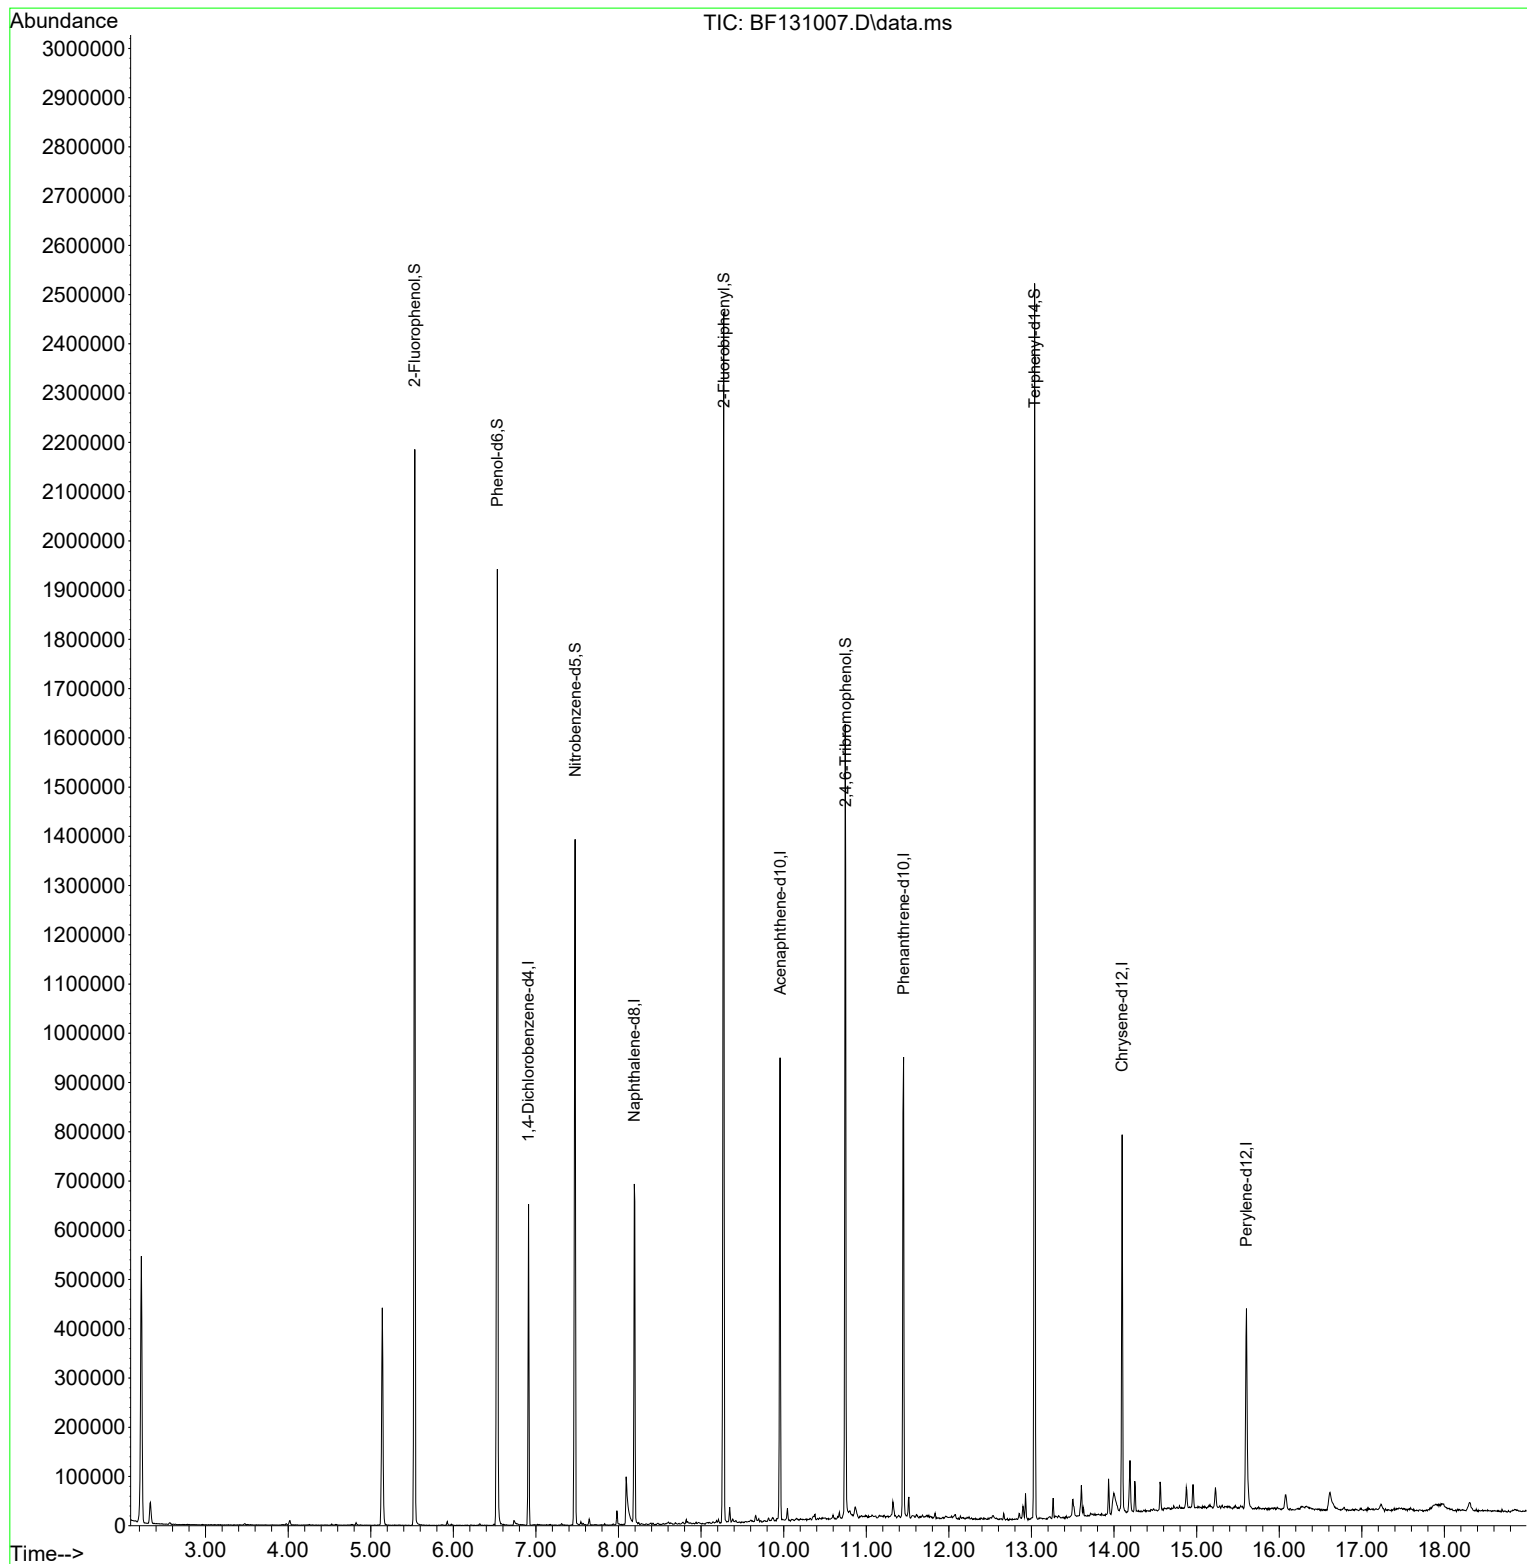




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.910 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10




Instrument :
BNA_F
ClientSampleId :
20221106-COMP-05


Tgt Ion:152 Resp: 80388
Ion Ratio Lower Upper
152 100
150 159.3 124.1 186.1
115 66.2 50.1 75.1

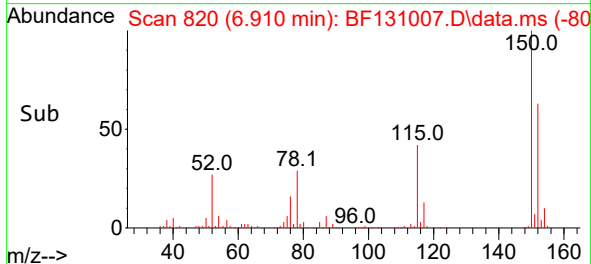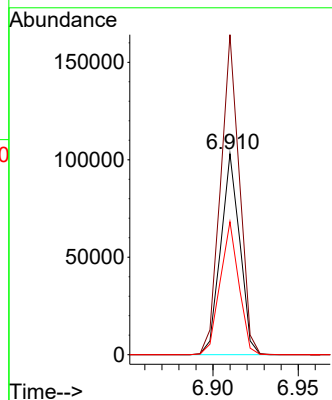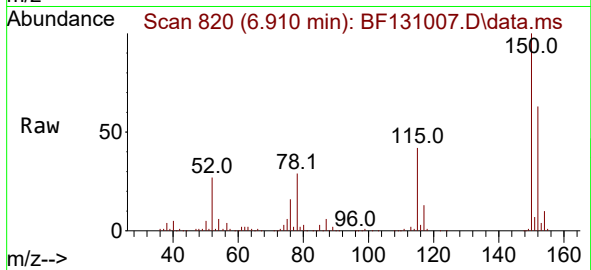

#5
2-Fluorophenol
Concen: 109.852 ng
RT: 5.534 min Scan# 586
Delta R.T. 0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10

Tgt Ion:112 Resp: 509385
Ion Ratio Lower Upper
112 100
64 67.4 53.9 80.9
63 37.7 29.4 44.2


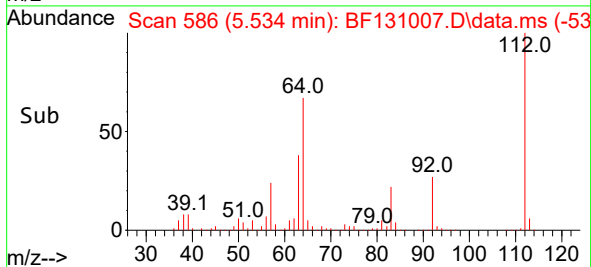
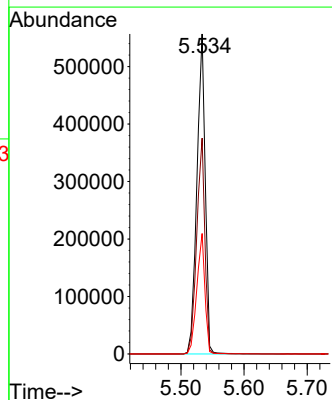
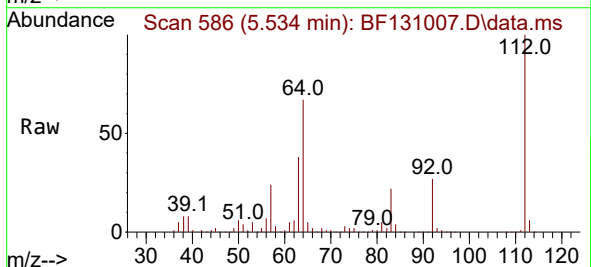


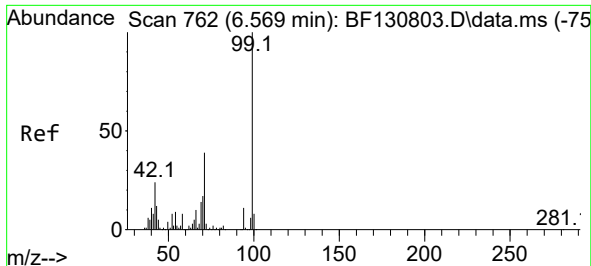

#7
Phenol-d6
Concen: 108.413 ng
RT: 6.534 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10




Instrument :
BNA_F
ClientSampleId :
20221106-COMP-05


Tgt Ion: 99 Resp: 653277
Ion Ratio Lower Upper
99 100
42 24.1 18.8 28.2
71 39.2 31.4 47.0

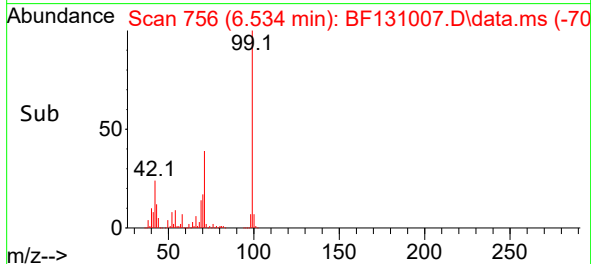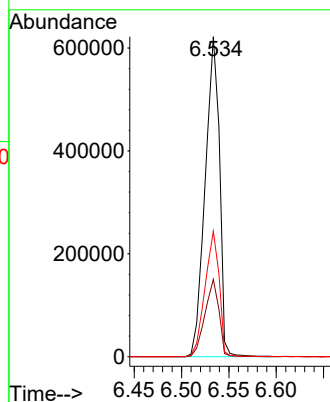

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.192 min Scan# 1038
Delta R.T. -0.012 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10

Tgt Ion: 136 Resp: 313849
Ion Ratio Lower Upper
136 100
137 10.7 9.2 13.8
54 10.0 8.8 13.2
68 6.0 5.2 7.8

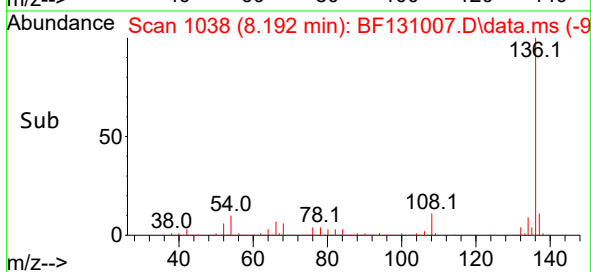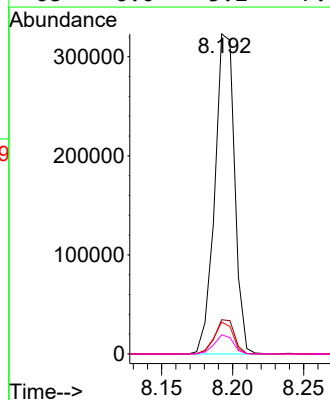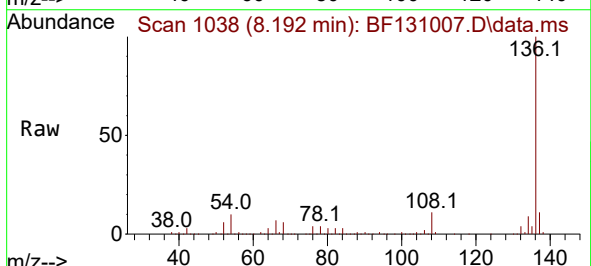

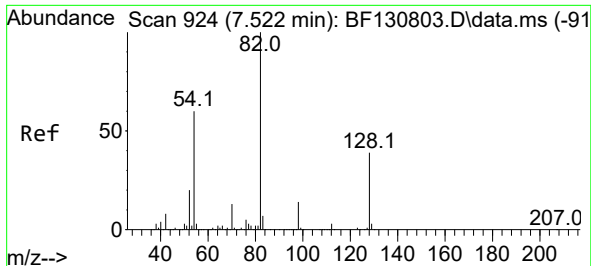

#23

Nitrobenzene-d5

Concen: 83.666 ng

RT: 7.475 min Scan# 91

Delta R.T. -0.012 min

Lab File: BF131007.D


Acq: 05 Nov 2022 00:10

Instrument :

BNA_F

ClientSampleId :

20221106-COMP-05






Tgt Ion: 82 Resp: 435475

Ion Ratio Lower Upper

82 100

128 40.6 31.2 46.8

54 57.4 48.0 72.0

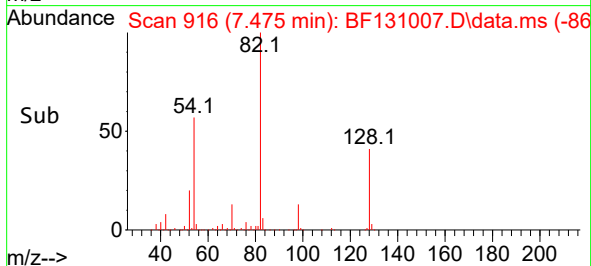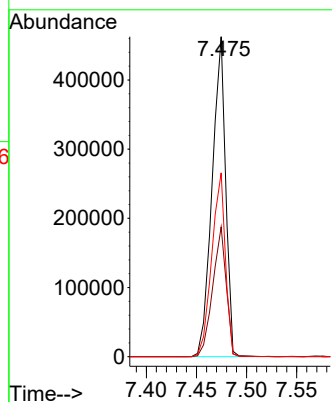

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.957 min Scan# 1338

Delta R.T. -0.006 min

Lab File: BF131007.D

Acq: 05 Nov 2022 00:10




Tgt Ion:164 Resp: 174469


Ion Ratio Lower Upper

164 100

162 97.7 82.2 123.2

160 45.2 36.6 54.8


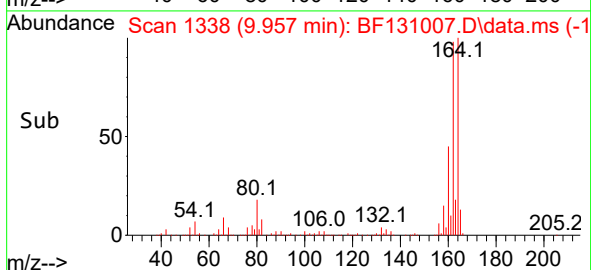
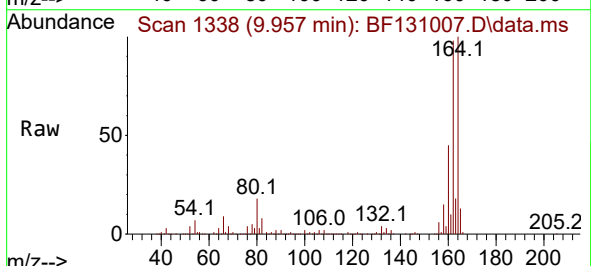
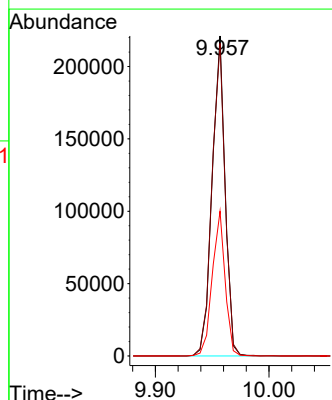




#42
2,4,6-Tribromophenol
Concen: 126.308 ng
RT: 10.751 min Scan# 1480
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10




Instrument :
BNA_F
ClientSampleId :
20221106-COMP-05


Tgt Ion:330 Resp: 185506
Ion Ratio Lower Upper
330 100
332 96.7 76.2 114.4
141 34.1 31.4 47.0

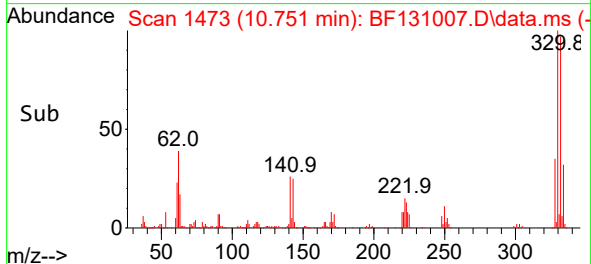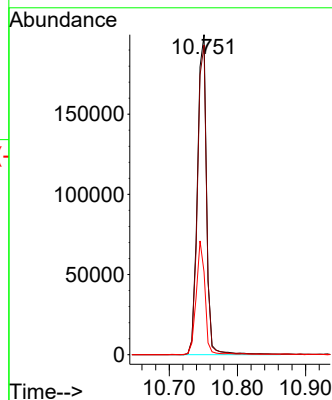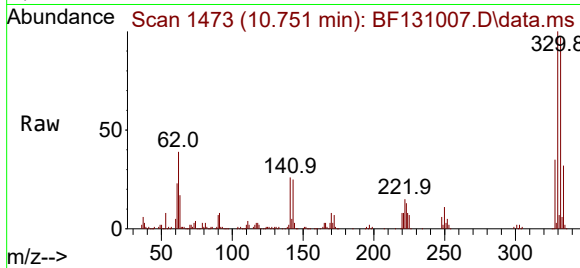

#45
2-Fluorobiphenyl
Concen: 64.461 ng
RT: 9.275 min Scan# 1222
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10

Tgt Ion:172 Resp: 743868
Ion Ratio Lower Upper
172 100
171 35.3 28.1 42.1
170 23.7 19.0 28.4


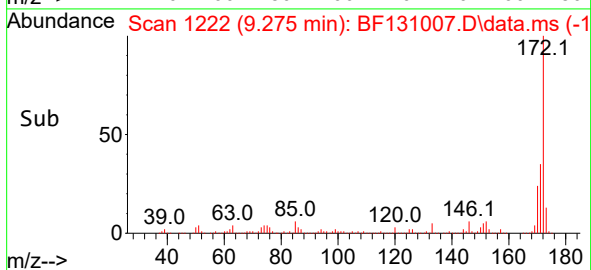
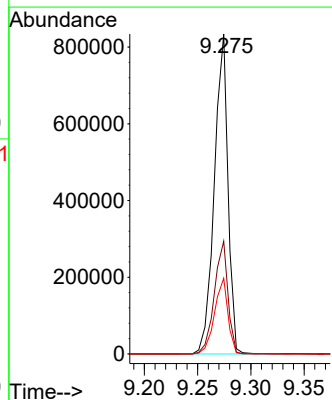
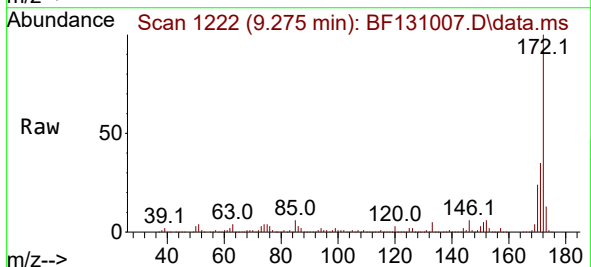


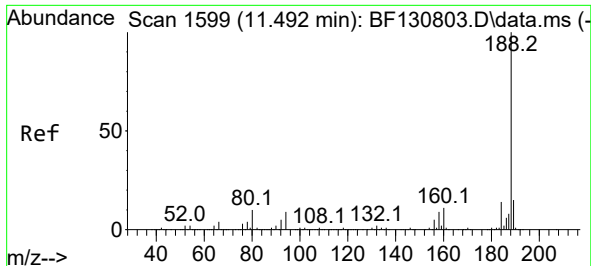

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10




Instrument :
BNA_F
ClientSampleId :
20221106-COMP-05


Tgt Ion:188 Resp: 335646
Ion Ratio Lower Upper
188 100
94 8.1 7.4 11.2
80 8.5 8.0 12.0

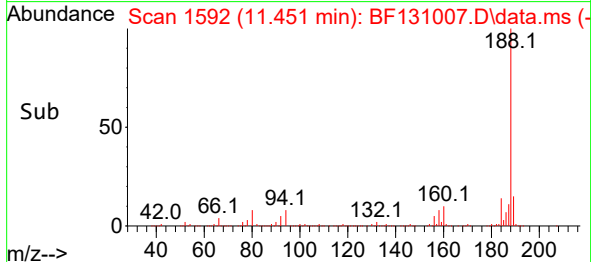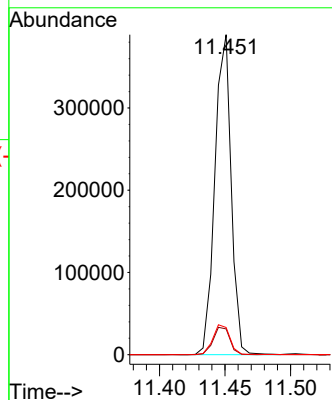

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.098 min Scan# 2042
Delta R.T. -0.006 min
Lab File: BF131007.D
Acq: 05 Nov 2022 00:10

Tgt Ion:240 Resp: 239489
Ion Ratio Lower Upper
240 100
120 9.5 7.0 10.4
236 24.8 20.5 30.7


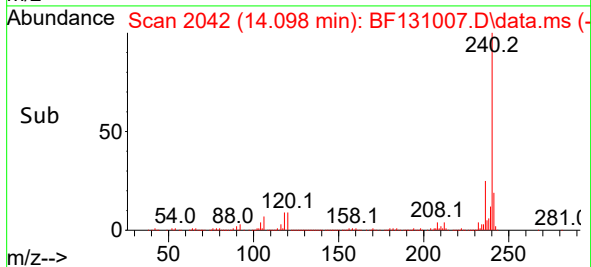
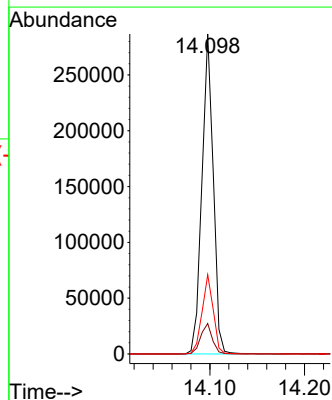
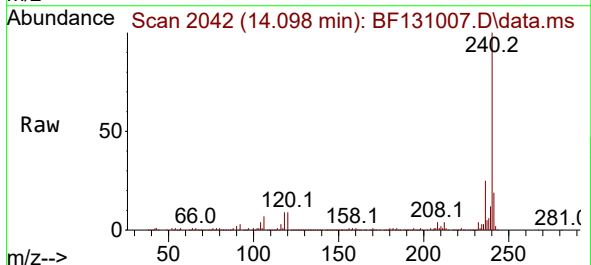


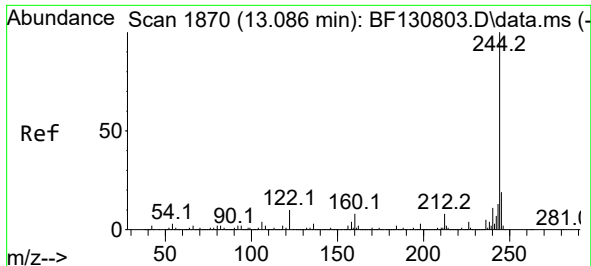

#79
 Terphenyl-d14
 Concen: 63.955 ng
 RT: 13.039 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF131007.D
 Acq: 05 Nov 2022 00:10

Instrument :
 BNA_F
 ClientSampleId :
 20221106-COMP-05

Tgt Ion:244 Resp: 835850
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.2
 122 10.5 7.9 11.9

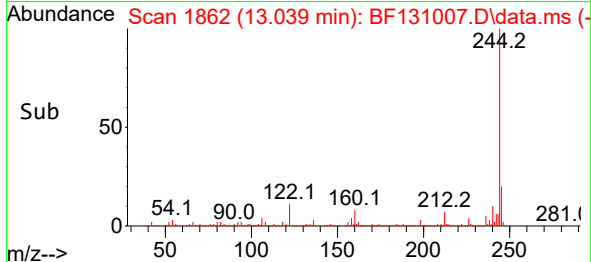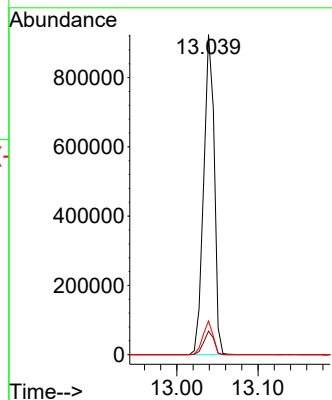

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.604 min Scan# 2298
 Delta R.T. -0.006 min
 Lab File: BF131007.D
 Acq: 05 Nov 2022 00:10

Tgt Ion:264 Resp: 184926
 Ion Ratio Lower Upper
 264 100
 260 22.9 19.9 29.9
 265 21.3 17.0 25.6

