

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF131006.D
 Acq On : 04 Nov 2022 23:37
 Operator : CG\JU
 Sample : N5310-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BIN 1-2-(2840)-COMP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	12	21	29	rVB	431401	596024	31.60%	4.394%
2	5.134	514	518	531	rVB	208359	257595	13.66%	1.899%
3	5.534	581	586	589	rBV	1651761	1664433	88.24%	12.270%
4	6.534	751	756	759	rBV	1828419	1669259	88.49%	12.306%
5	6.910	816	820	824	rBV	585020	449918	23.85%	3.317%
6	7.475	911	916	919	rBV	1239624	1115444	59.13%	8.223%
7	8.104	1018	1023	1034	rBV4	22992	61609	3.27%	0.454%
8	8.192	1034	1038	1042	rVV	623783	565974	30.00%	4.172%
9	9.275	1217	1222	1225	rBV	2113164	1886285	100.00%	13.906%
10	9.957	1334	1338	1341	rBV	697071	585637	31.05%	4.317%
11	10.745	1468	1472	1487	rVB	1097294	944270	50.06%	6.961%
12	11.445	1588	1591	1594	rBV	662227	602758	31.95%	4.444%
13	11.516	1600	1603	1607	rVB3	28616	25138	1.33%	0.185%
14	12.663	1795	1798	1801	rVB	39485	33931	1.80%	0.250%
15	12.892	1832	1837	1841	rBV	38285	41985	2.23%	0.310%
16	13.039	1858	1862	1865	rBV	1990389	1683210	89.23%	12.409%
17	14.004	2018	2026	2035	rBV6	37705	128737	6.82%	0.949%
18	14.098	2038	2042	2045	rBV	549057	477347	25.31%	3.519%
19	14.192	2053	2058	2066	rBV	112260	131130	6.95%	0.967%
20	14.874	2171	2174	2179	rBV2	20741	23521	1.25%	0.173%
21	15.157	2218	2222	2230	rBV3	20487	42132	2.23%	0.311%
22	15.227	2231	2234	2238	rVB	24572	25935	1.37%	0.191%
23	15.533	2283	2286	2289	rBV	15845	20977	1.11%	0.155%
24	15.604	2292	2298	2308	rBV	374782	509896	27.03%	3.759%
25	16.074	2376	2378	2386	rVB4	13429	21417	1.14%	0.158%




Sum of corrected areas: 13564562

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF131006.D
Acq On : 04 Nov 2022 23:37
Operator : CG\JU
Sample : N5310-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BIN 1-2-(2840)-COMP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

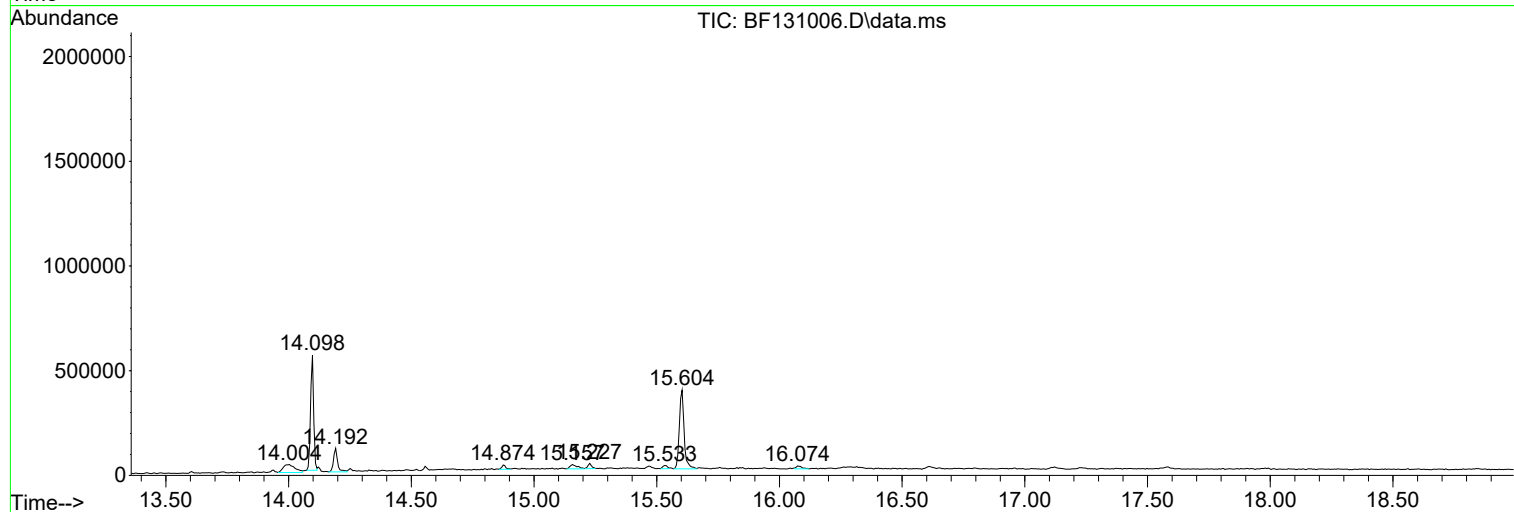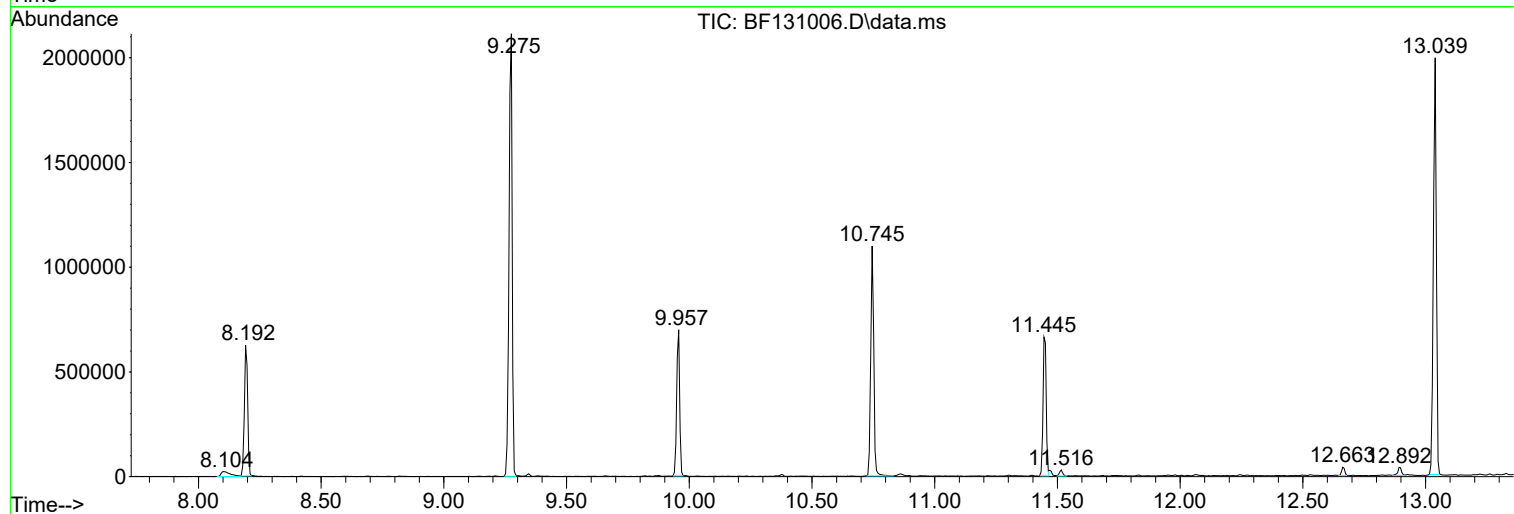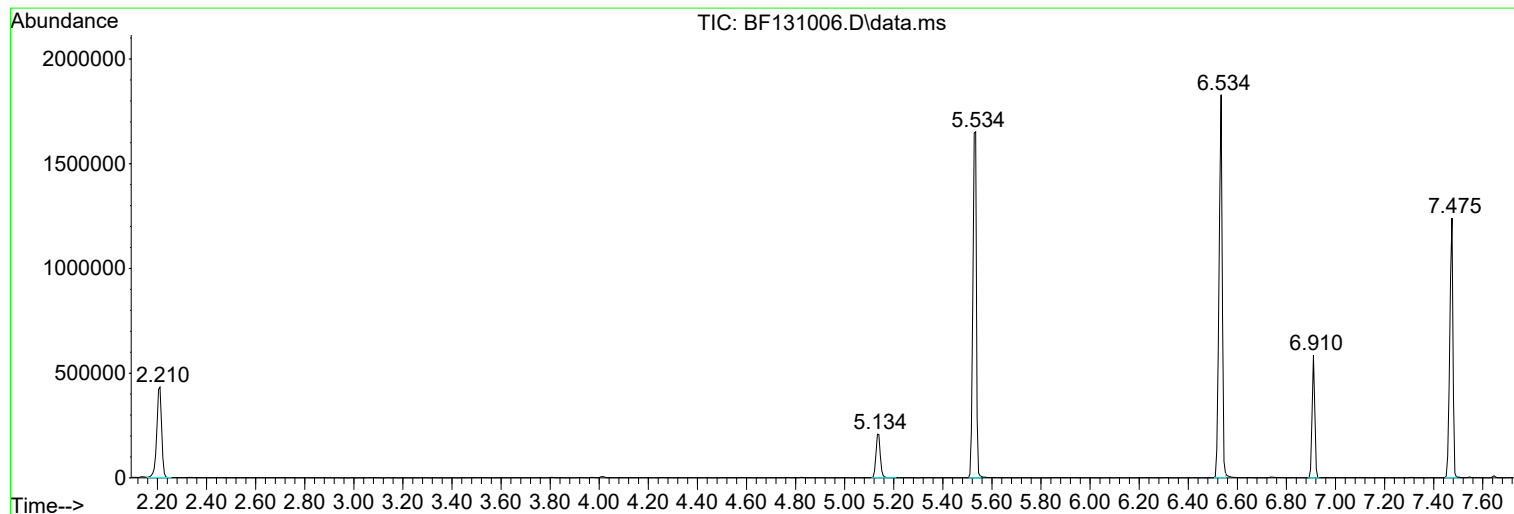

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF131006.D
Acq On : 04 Nov 2022 23:37
Operator : CG\JU
Sample : N5310-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BIN 1-2-(2840)-COMP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF131006.D
Acq On : 04 Nov 2022 23:37
Operator : CG\JU
Sample : N5310-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BIN 1-2-(2840)-COMP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------