
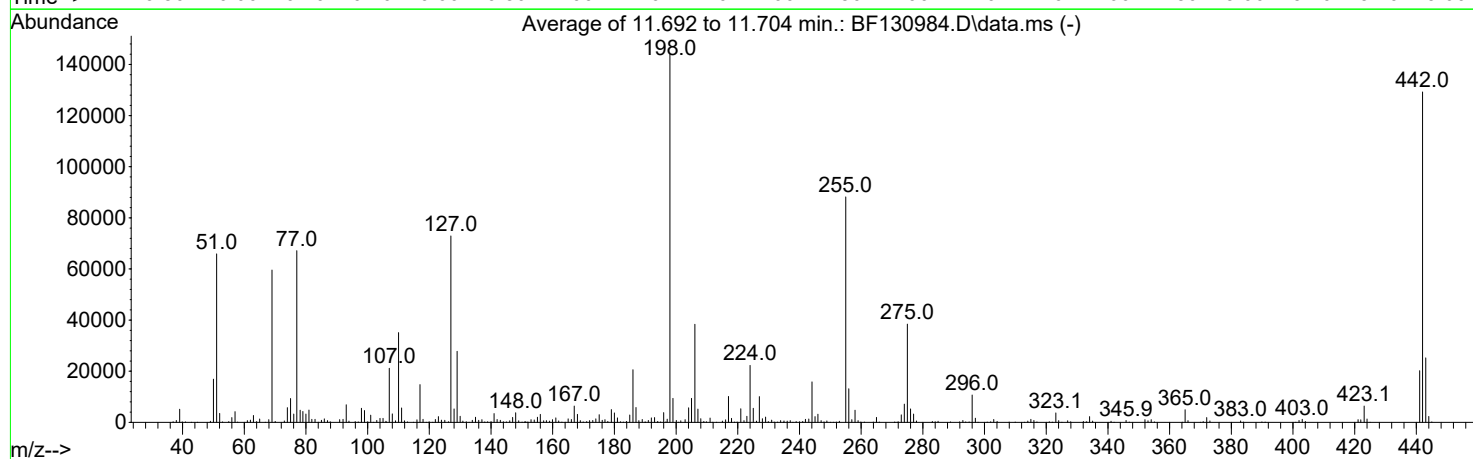


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF130984.D
 Acq On : 04 Nov 2022 10:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:46:02 2022

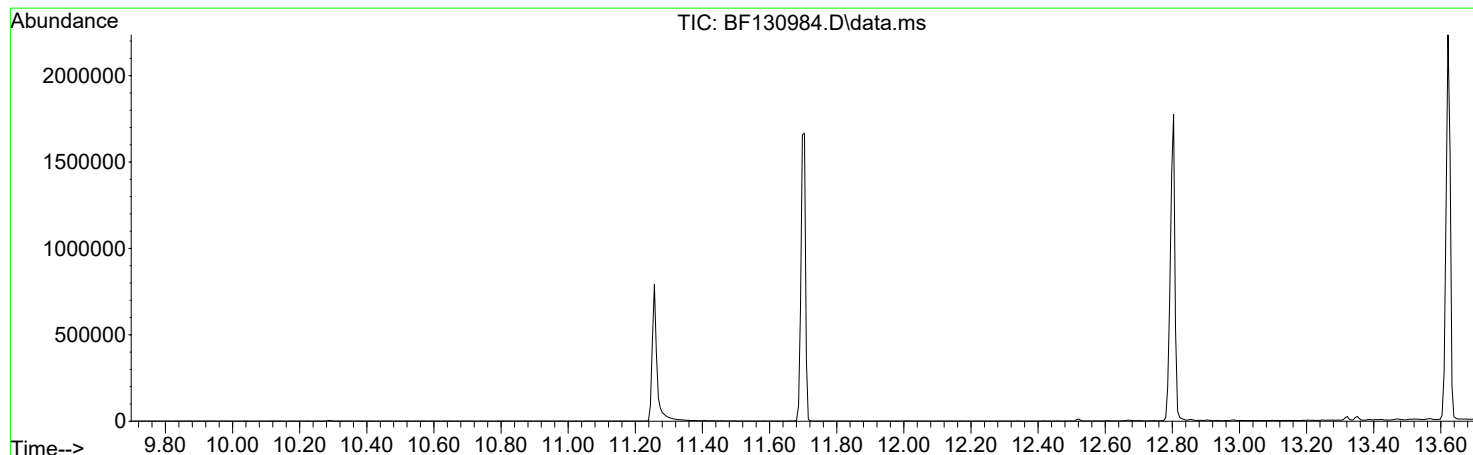




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	65899	PASS
68	69	0.00	2	1.8	1074	PASS
69	198	0.00	100	41.4	59568	PASS
70	69	0.00	2	0.6	362	PASS
127	198	10	80	50.7	72941	PASS
197	198	0.00	2	0.9	1266	PASS
198	198	100	100	100.0	143885	PASS
199	198	5	9	6.5	9397	PASS
275	198	10	60	26.7	38412	PASS
365	198	1	100	3.4	4957	PASS
441	198	0.01	100	14.1	20236	PASS
442	442	50	100	100.0	129256	PASS
443	442	15	24	19.5	25198	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130984.D
Acq On : 04 Nov 2022 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 04:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

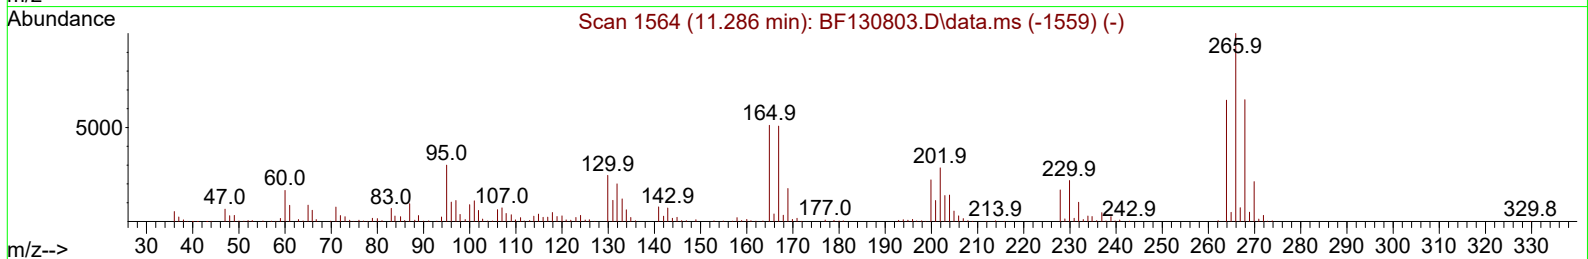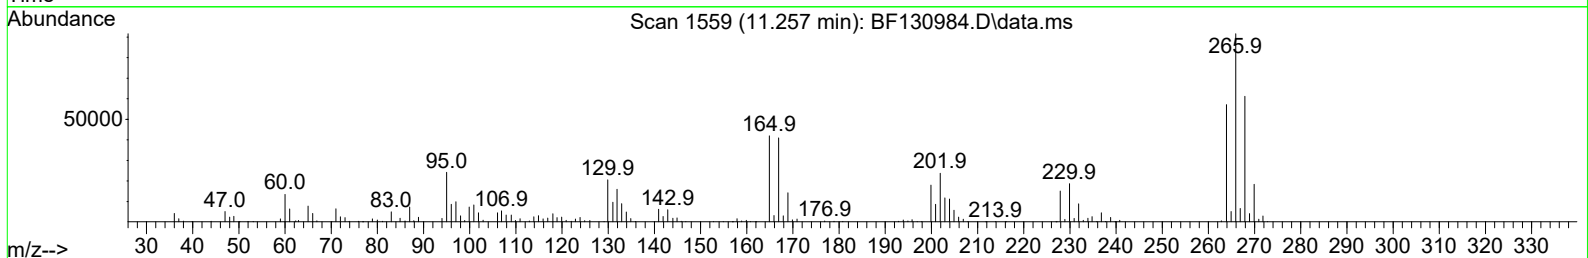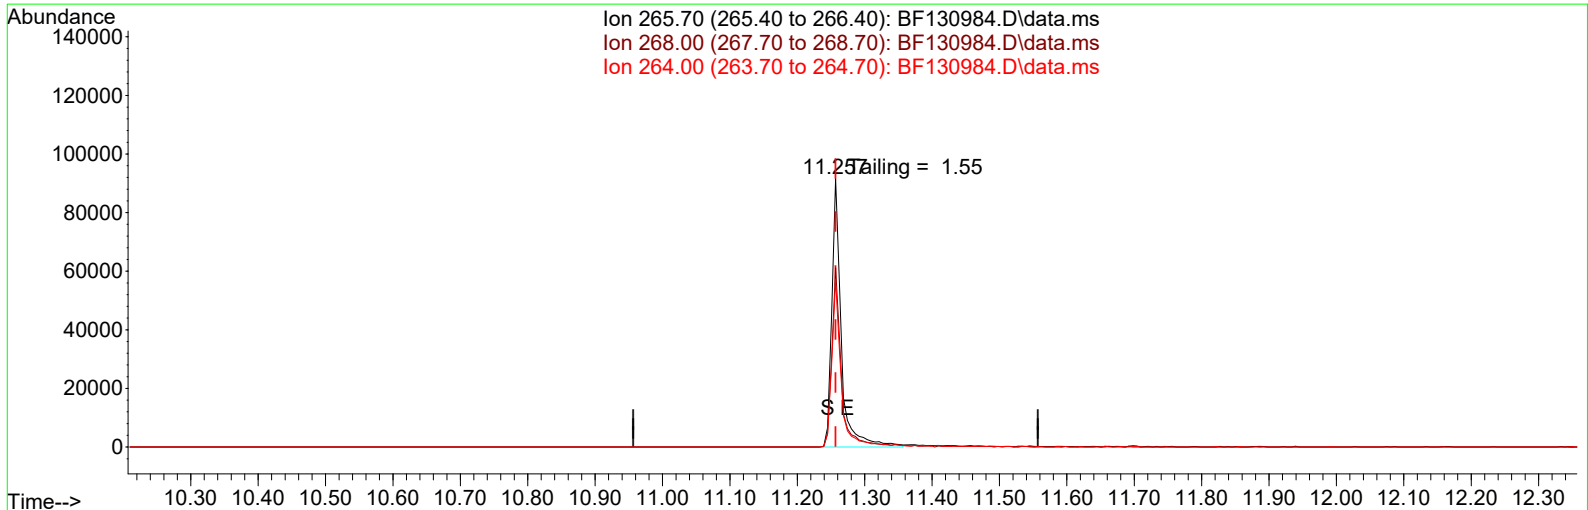

TIC: BF130984.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 19243.67 ng




response 90159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.79
264.00	64.50	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130984.D
Acq On : 04 Nov 2022 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 04:13:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

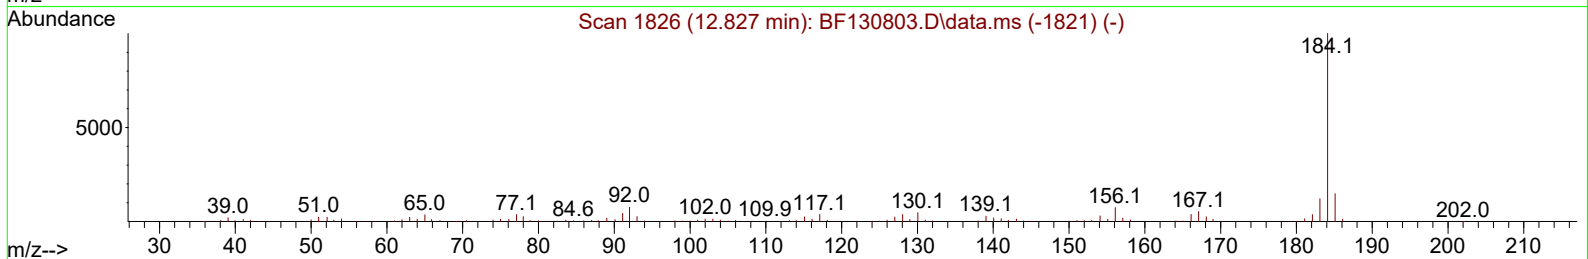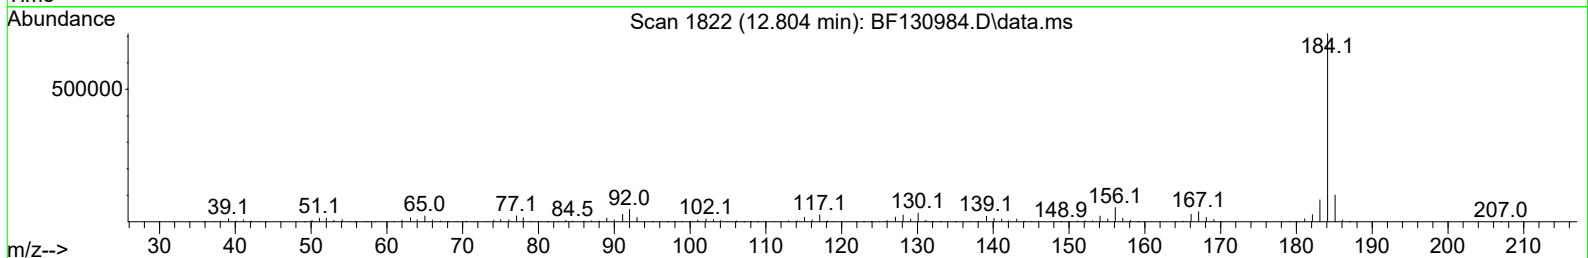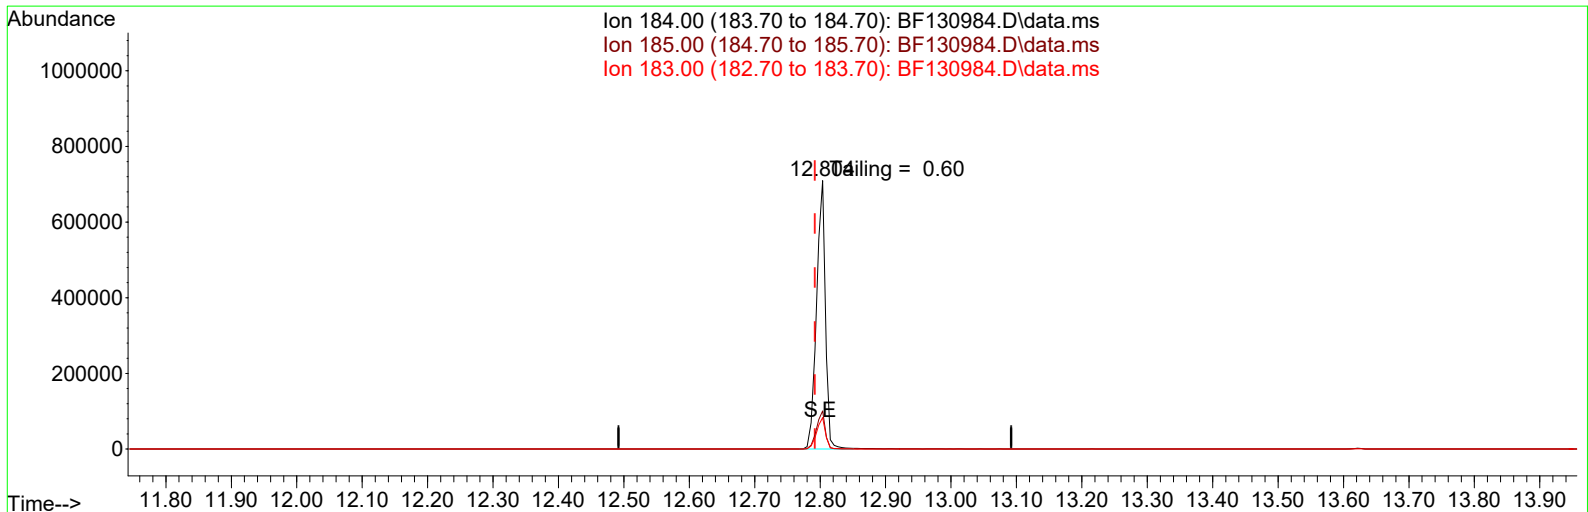

TIC: BF130984.D\data.ms

(77) Benzidine

12.804min (+ 0.012) 479347.71 ng

response 674896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.19
183.00	12.10	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2022	BNA_F	BF130984.D
Compound Name	Response	Retention Time
DDT	377579	13.621
DDD	7384	13.321
DDE	720	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8104	385683	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP