
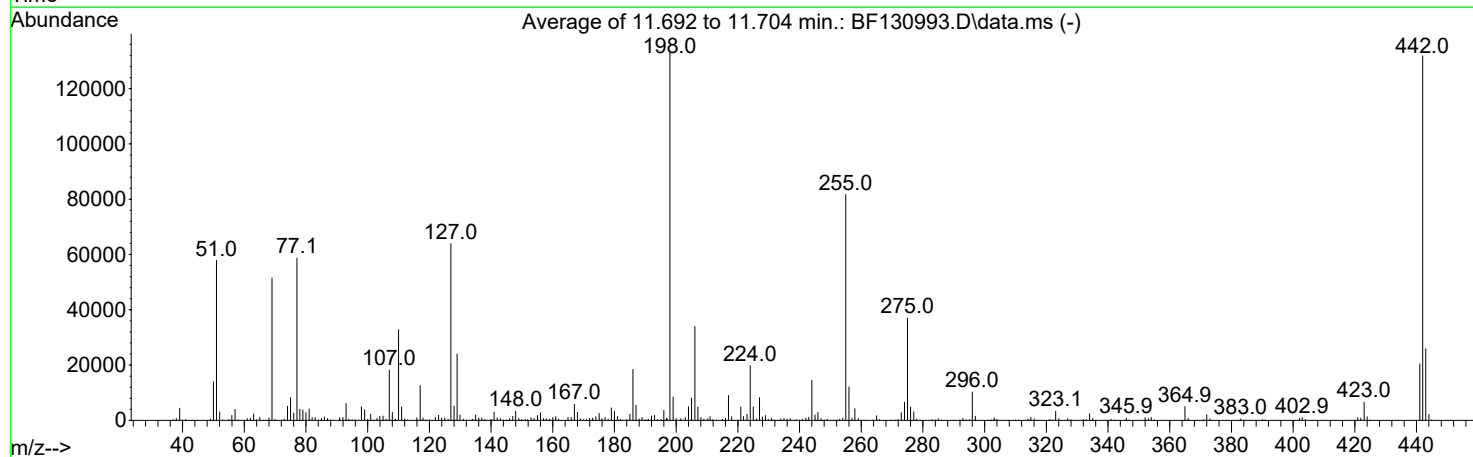


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF130993.D
 Acq On : 04 Nov 2022 15:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 07 00:46:02 2022

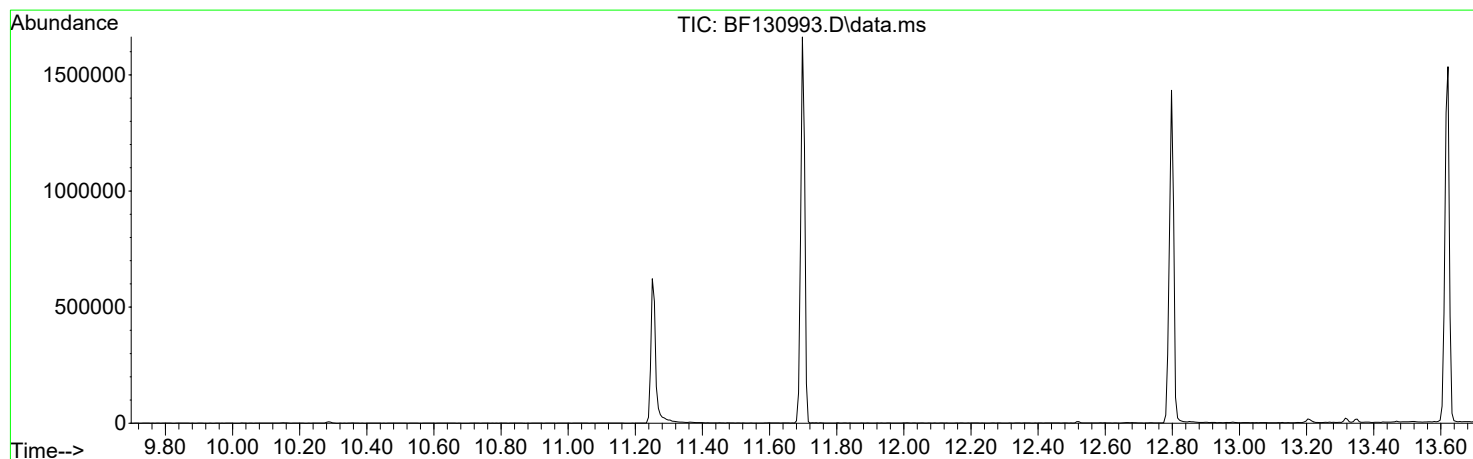




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	57856	PASS
68	69	0.00	2	1.6	808	PASS
69	198	0.00	100	38.7	51555	PASS
70	69	0.00	2	0.6	295	PASS
127	198	10	80	48.1	63973	PASS
197	198	0.00	2	0.5	690	PASS
198	198	100	100	100.0	133069	PASS
199	198	5	9	6.3	8449	PASS
275	198	10	60	27.8	36955	PASS
365	198	1	100	3.8	4999	PASS
441	198	0.01	100	15.3	20420	PASS
442	442	50	100	100.0	131933	PASS
443	442	15	24	19.7	25945	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
Data File : BF130993.D
Acq On : 04 Nov 2022 15:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 05 04:15:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 06:20:24 2022
Response via : Initial Calibration

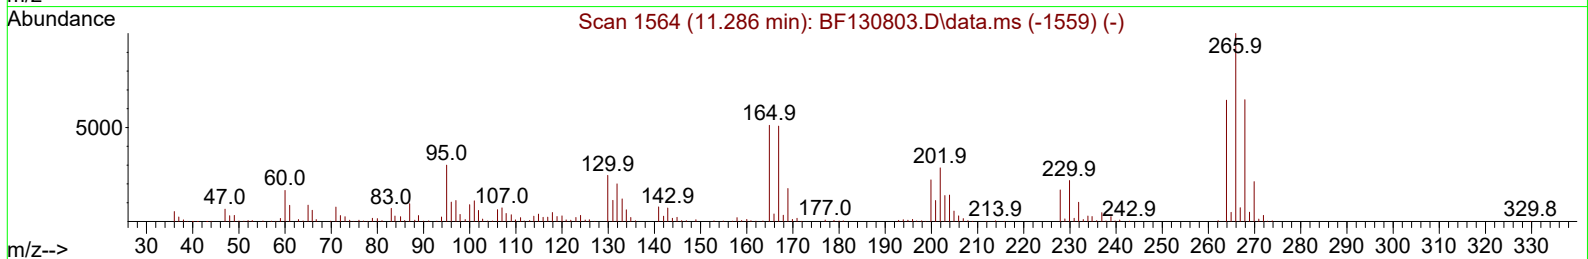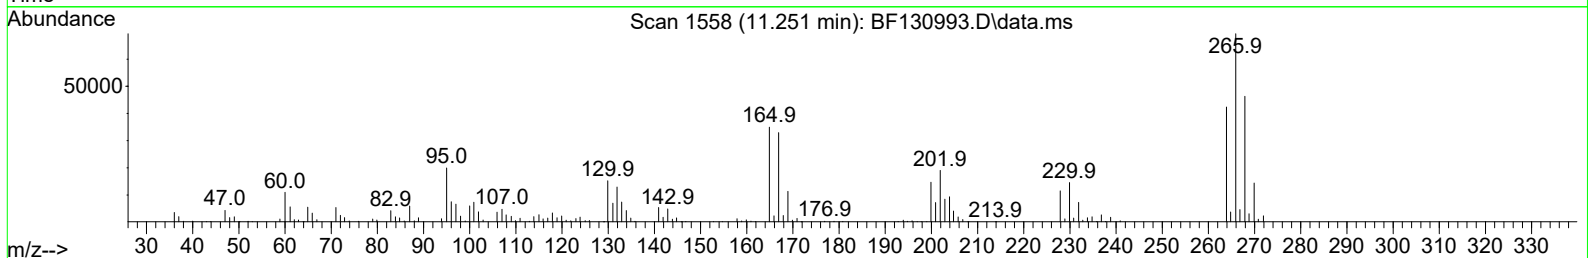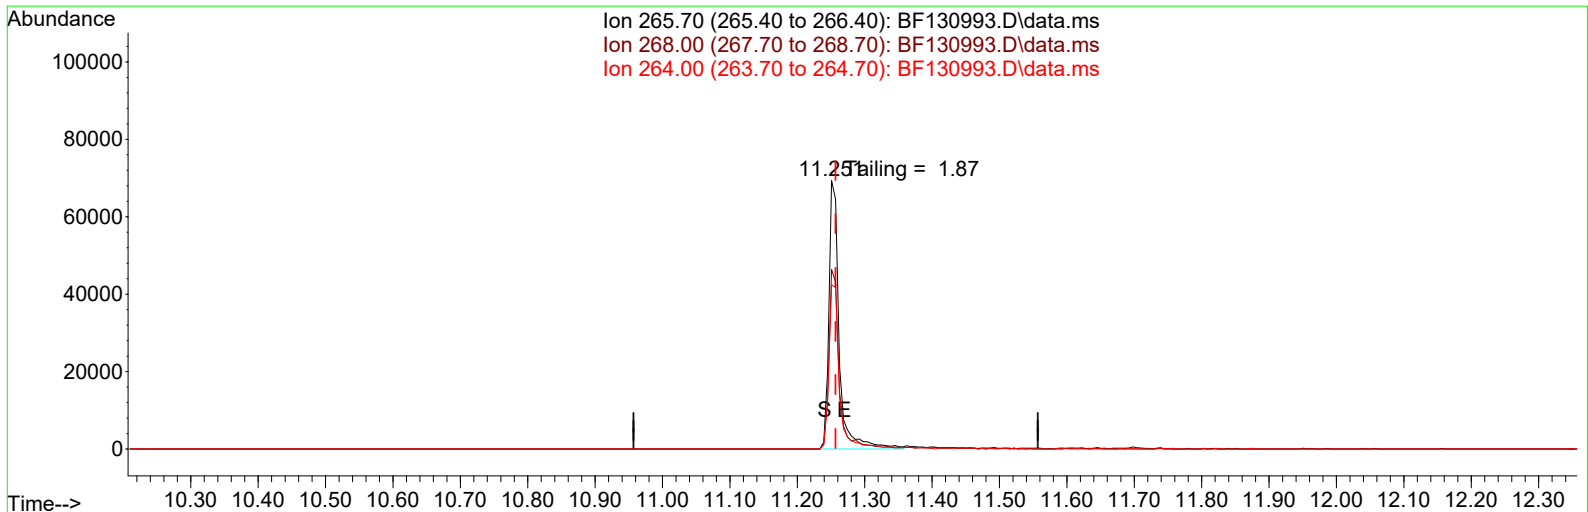

TIC: BF130993.D\data.ms

(70) Pentachlorophenol (C)

11.251min (-0.006) 20340.32 ng




response 74077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.82
264.00	64.50	61.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110422\
 Data File : BF130993.D
 Acq On : 04 Nov 2022 15:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 05 04:15:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 06:20:24 2022
 Response via : Initial Calibration

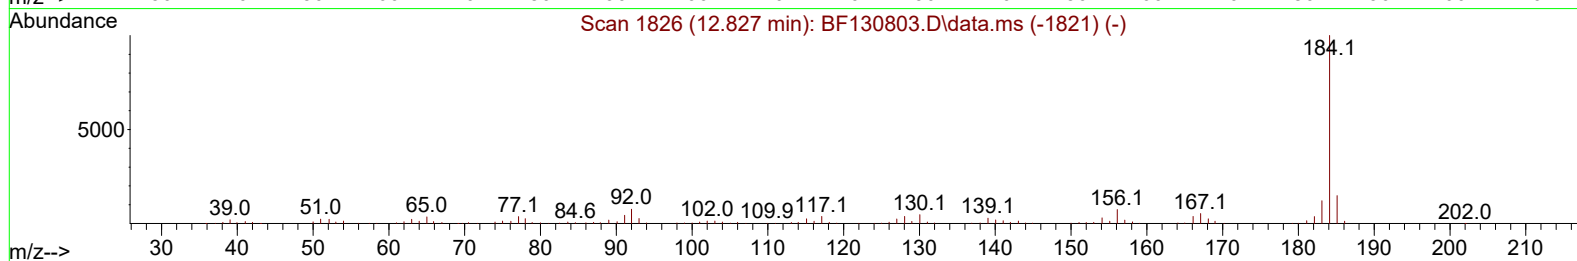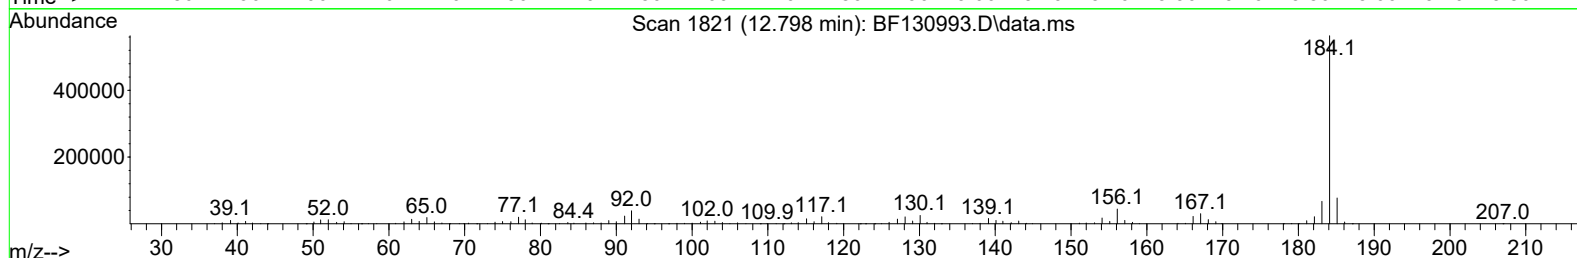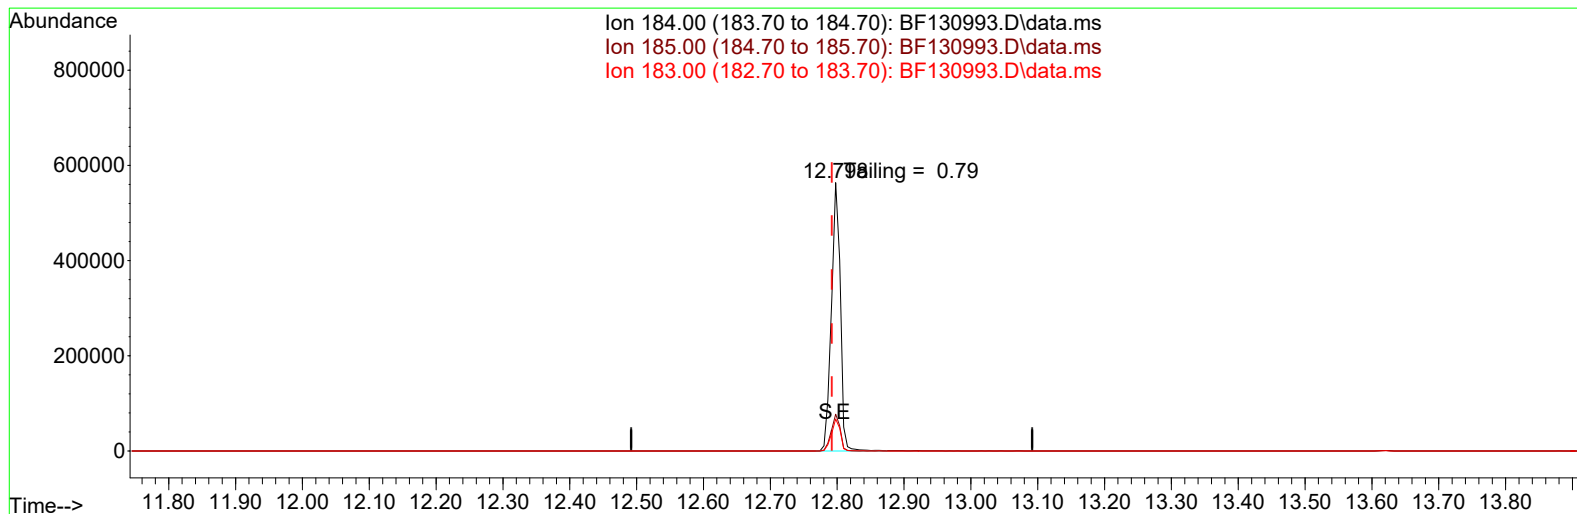

TIC: BF130993.D\data.ms

(77) Benzidine

12.798min (+ 0.006) 0.00 ng

response 525611

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.72
183.00	12.10	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2022	BNA_F	BF130993.D
Compound Name	Response	Retention Time
DDT	265656	13.621
DDD	5821	13.315
DDE	406	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6227	271883	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP