
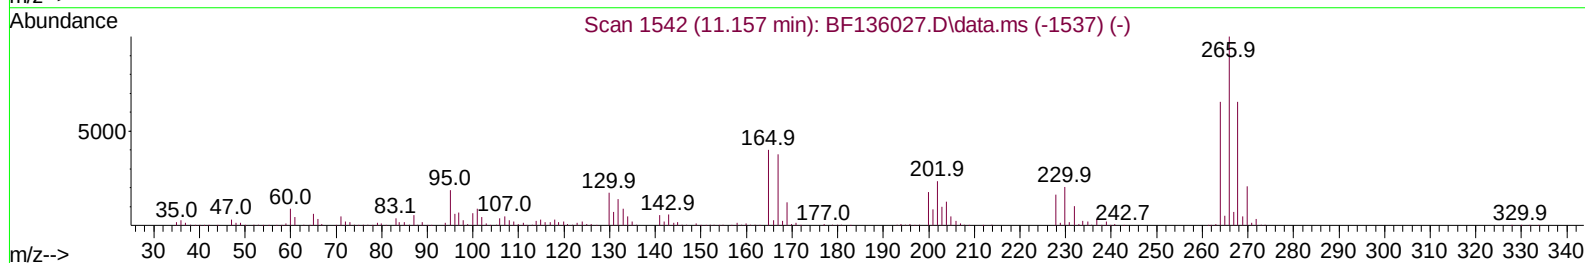
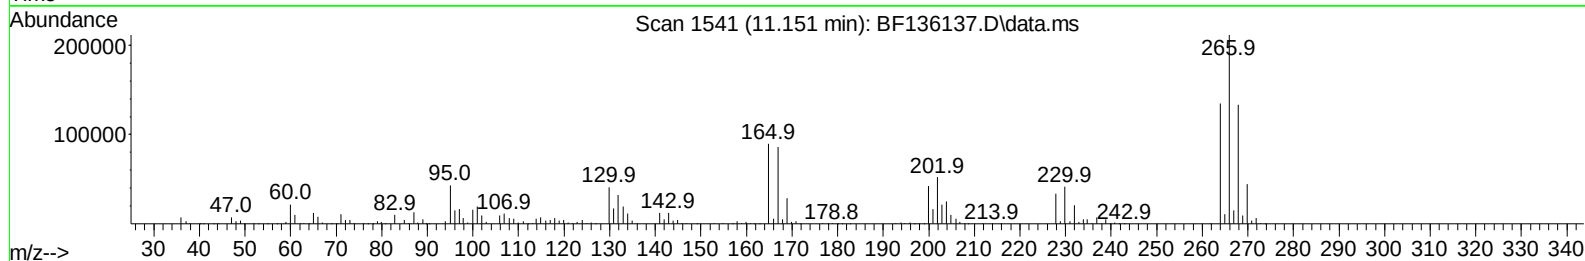


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136137.D
Acq On : 04 Nov 2023 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 01:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

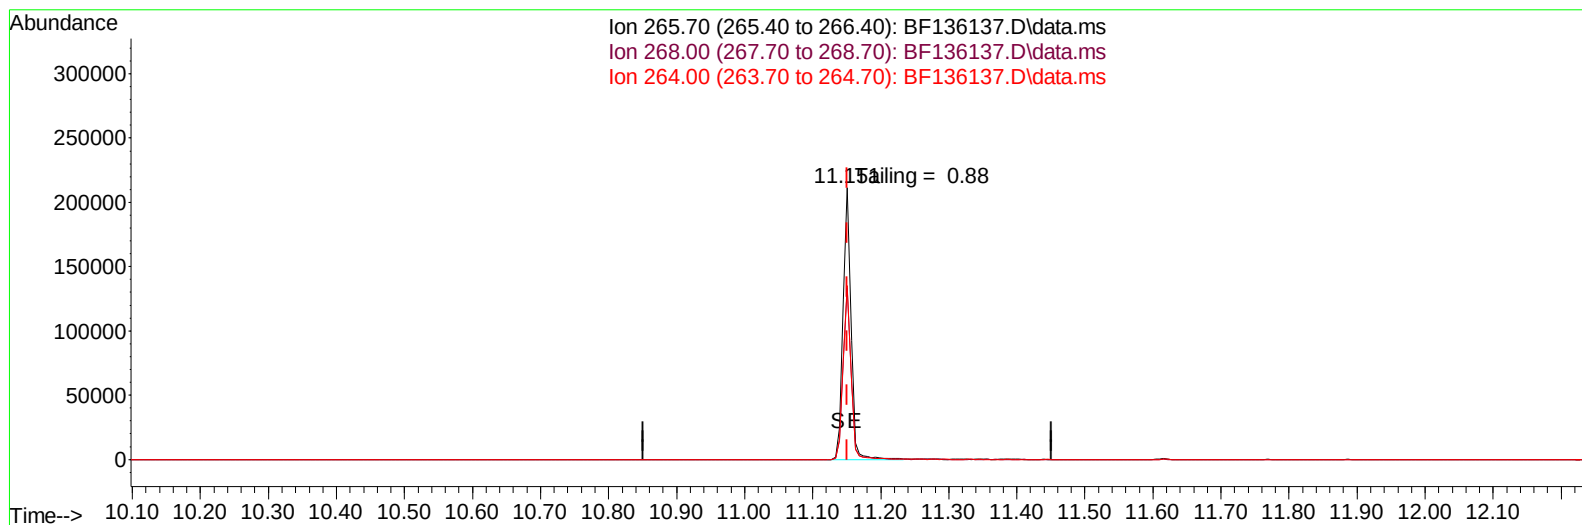

TIC: BF136137.D\data.ms




(70) Pentachlorophenol (C)

11.151min (+ 0.000) 283615.11 ng

response 171321

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.18
264.00	65.30	63.91
0.00	0.00	0.00

Quant Time: Nov 06 01:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

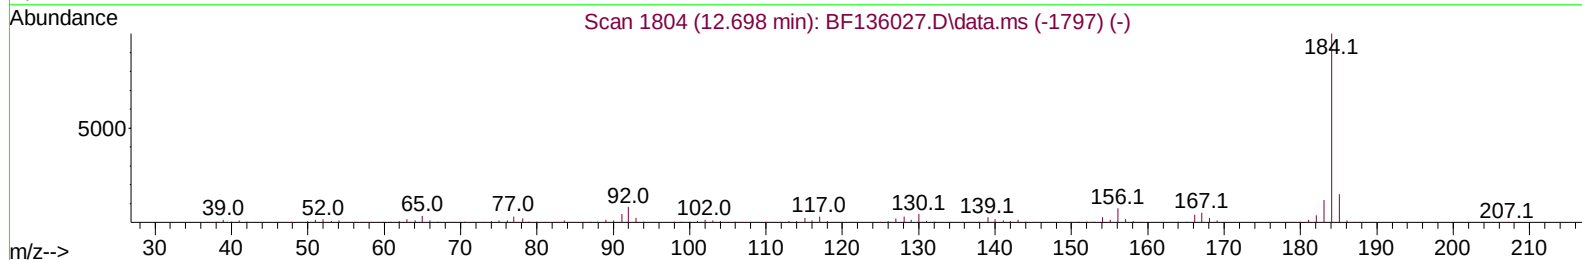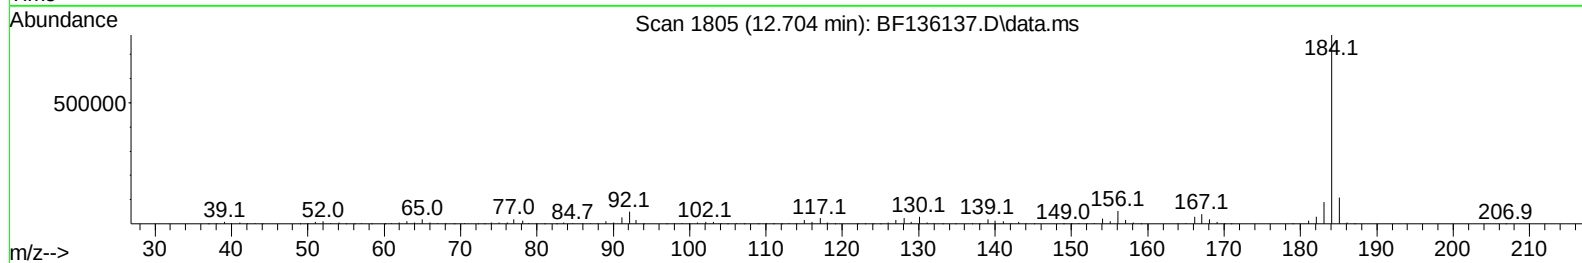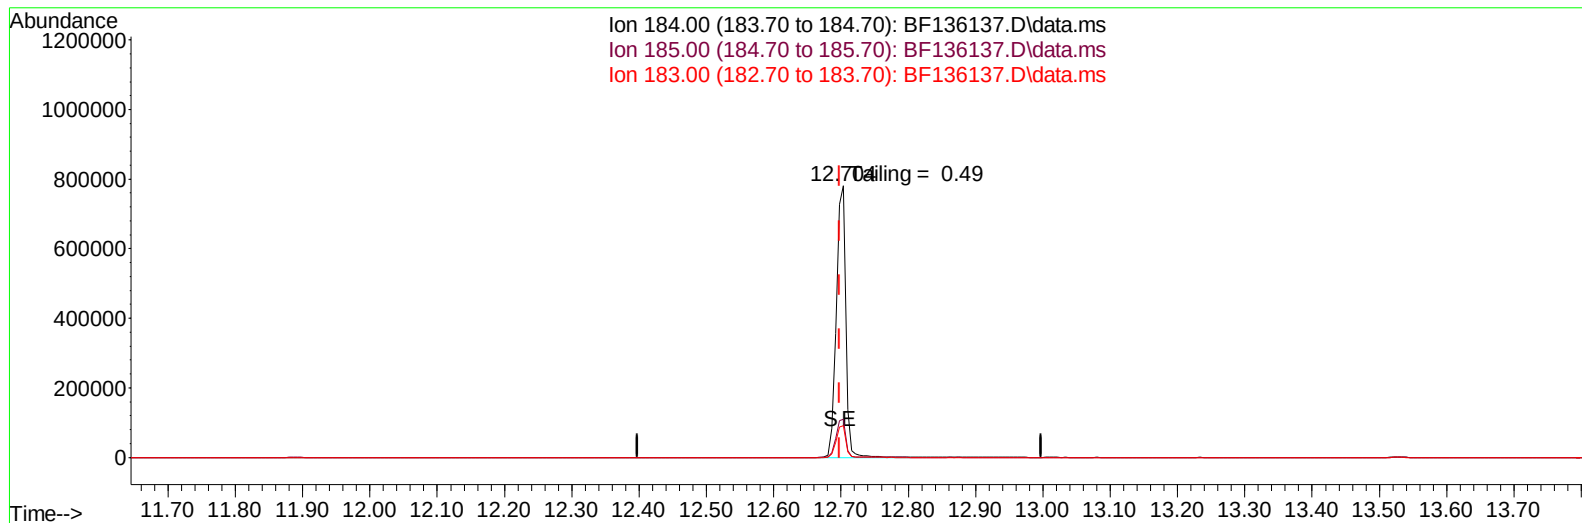

TIC: BF136137.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 285948.45 ng

response **763552**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.01
183.00	11.90	11.71
0.00	0.00	0.00