

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
 Data File : BF136146.D
 Acq On : 04 Nov 2023 14:27
 Operator : CG\JU
 Sample : 05242-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-303-20231102

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	566	570	573	rBV	1075806	901213	28.57%	6.150%
2	6.440	736	740	743	rBV	659844	506272	16.05%	3.455%
3	6.816	801	804	808	rBV	717660	542090	17.18%	3.699%
4	7.381	895	900	903	rBV	1802071	1638172	51.93%	11.179%
5	8.098	1018	1022	1025	rBV	938448	714048	22.63%	4.873%
6	9.181	1202	1206	1209	rBV	3799933	3154694	100.00%	21.527%
7	9.857	1317	1321	1324	rBV	1013583	816624	25.89%	5.572%
8	10.651	1451	1456	1459	rBV	1965241	1897789	60.16%	12.950%
9	11.345	1570	1574	1578	rBV	966354	795630	25.22%	5.429%
10	12.951	1842	1847	1850	rBV	2955653	2564775	81.30%	17.502%
11	14.004	2022	2026	2037	rBV	557414	497079	15.76%	3.392%
12	15.492	2273	2279	2287	rBV	500963	626171	19.85%	4.273%




Sum of corrected areas: 14654557

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136146.D
Acq On : 04 Nov 2023 14:27
Operator : CG\JU
Sample : 05242-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

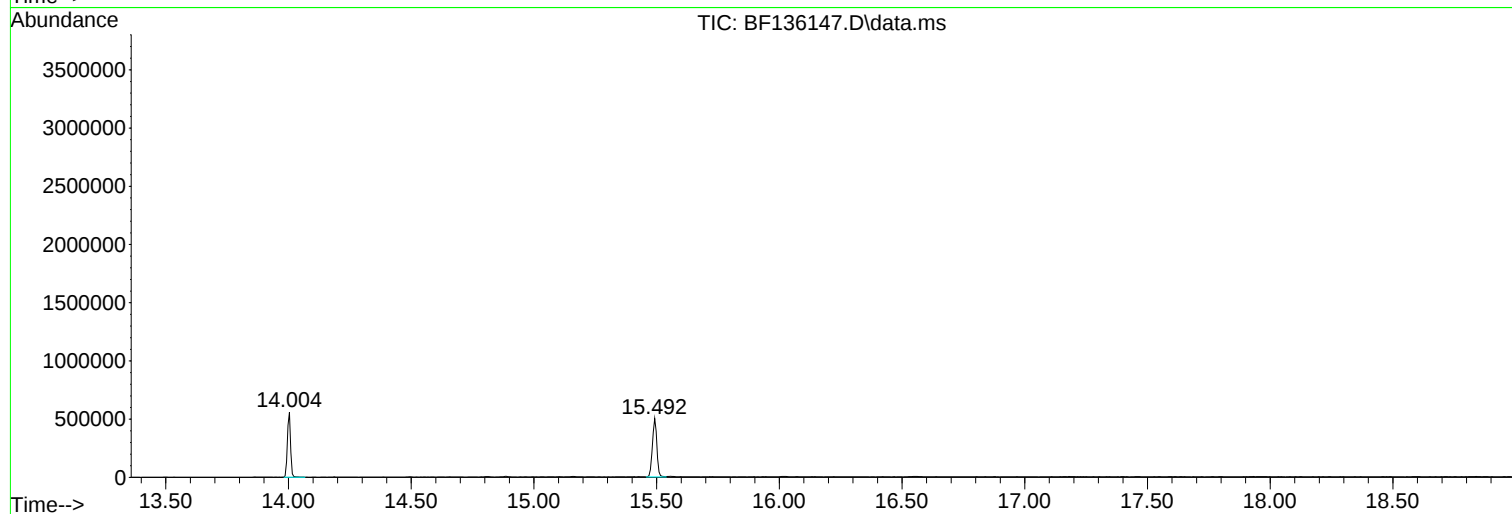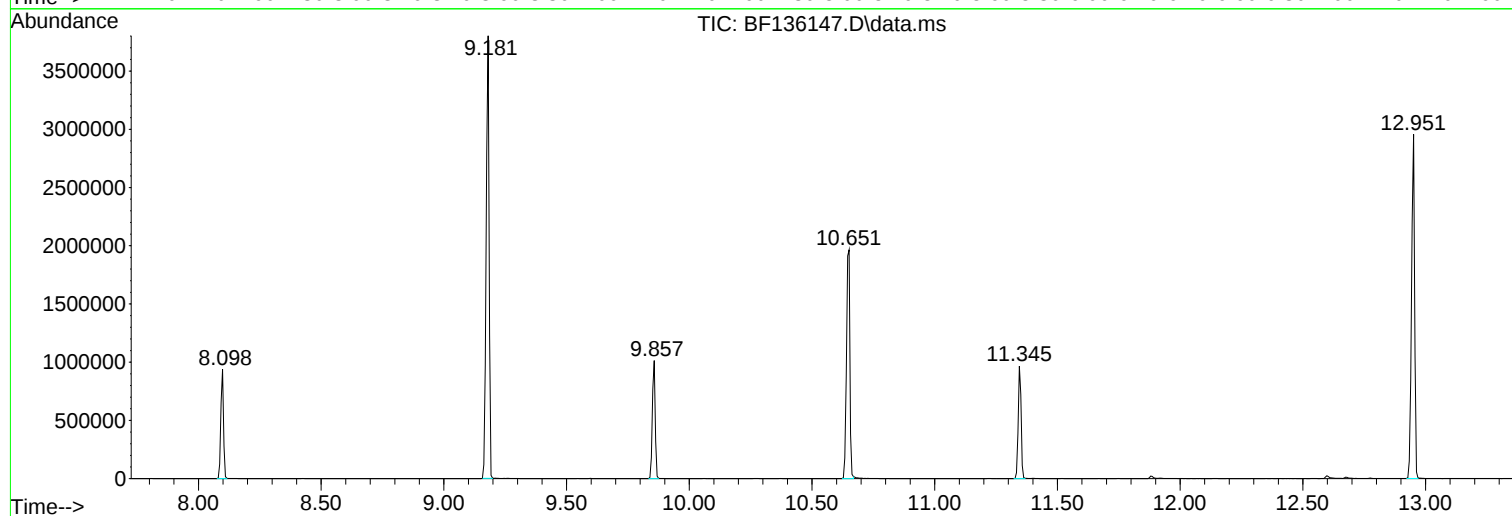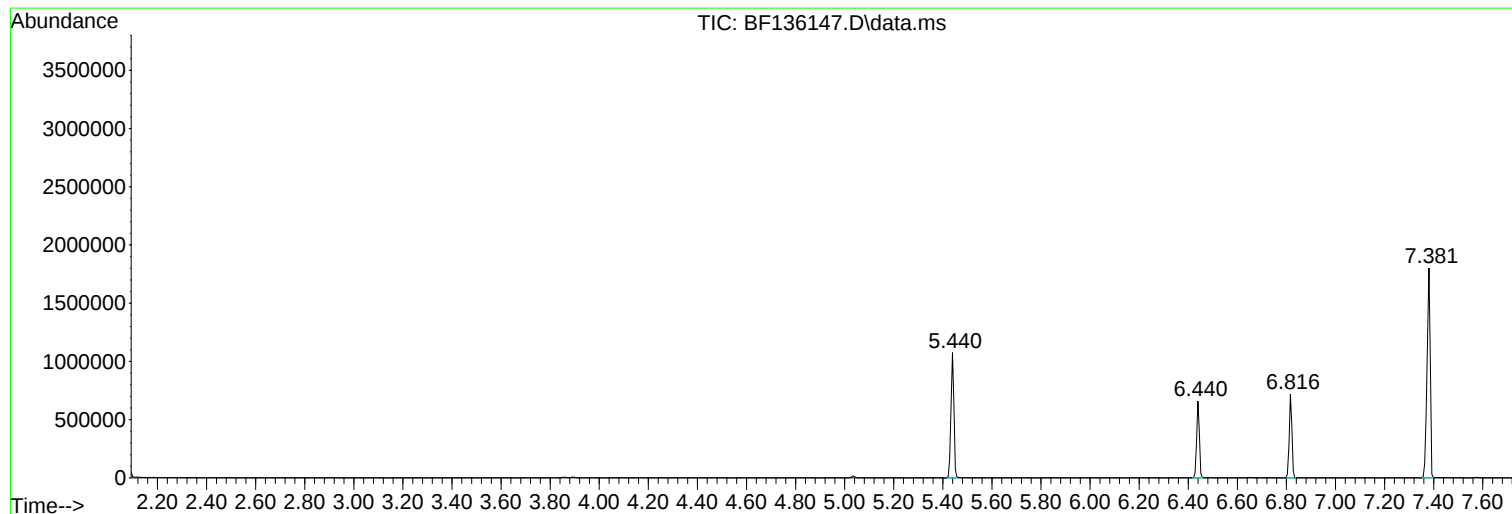

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136146.D
Acq On : 04 Nov 2023 14:27
Operator : CG\JU
Sample : 05242-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136146.D
Acq On : 04 Nov 2023 14:27
Operator : CG\JU
Sample : 05242-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20231102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------