


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136137.D
Acq On : 04 Nov 2023 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 06 00:53:35 2023

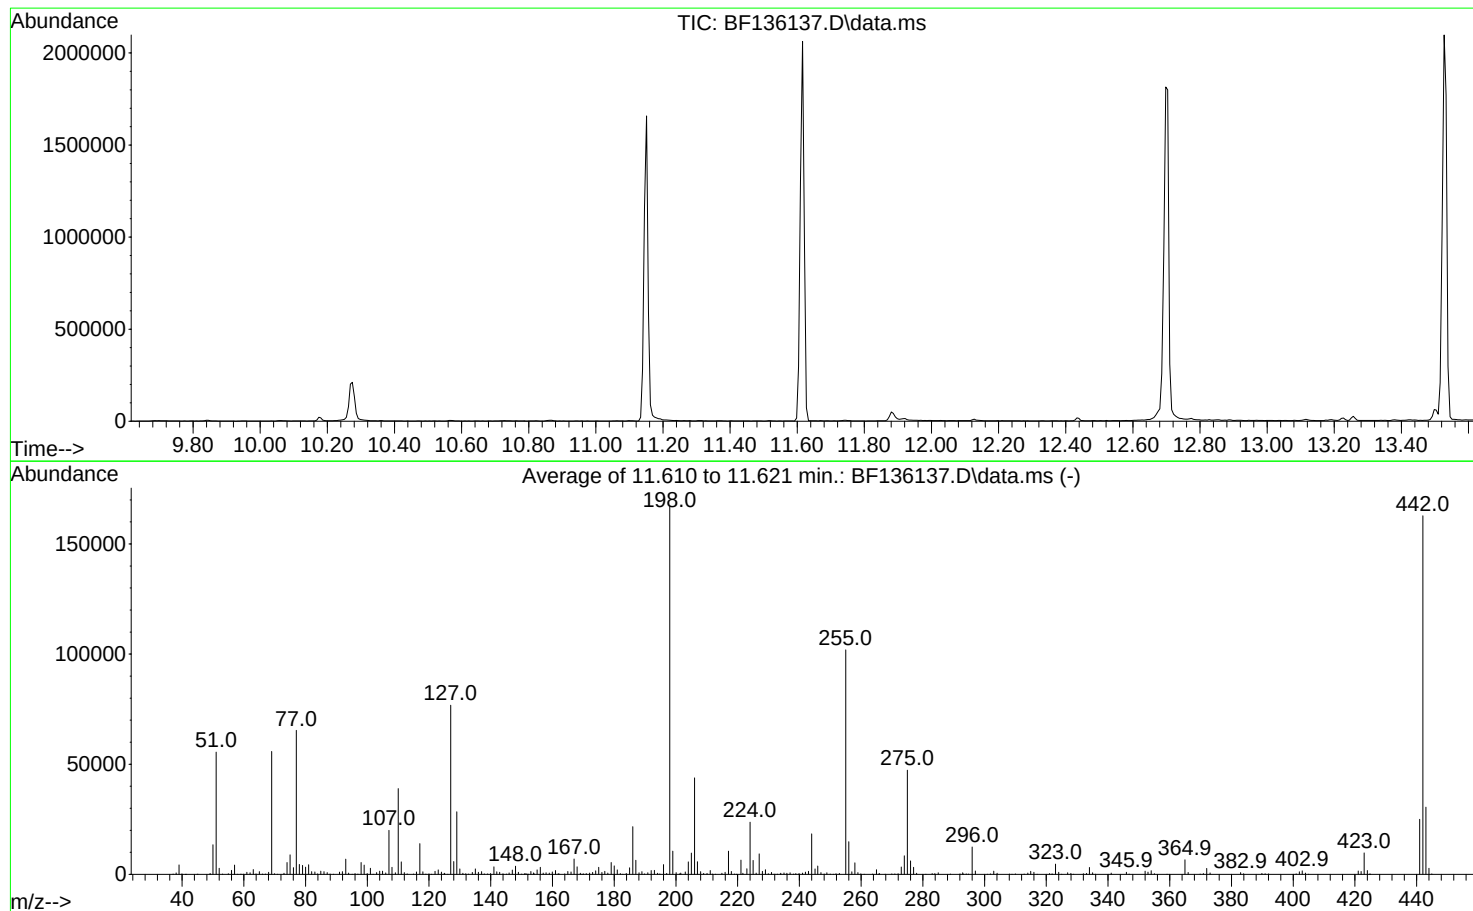




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	55533	PASS
68	69	0.00	2	1.8	977	PASS
69	198	0.00	100	33.4	55811	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	46.0	76808	PASS
197	198	0.00	2	0.2	410	PASS
198	198	100	100	100.0	167000	PASS
199	198	5	9	6.3	10569	PASS
275	198	10	60	28.3	47264	PASS
365	198	1	100	3.9	6586	PASS
441	198	0.01	100	15.0	25025	PASS
442	442	50	100	100.0	162821	PASS
443	442	15	24	18.7	30488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136137.D
Acq On : 04 Nov 2023 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 01:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

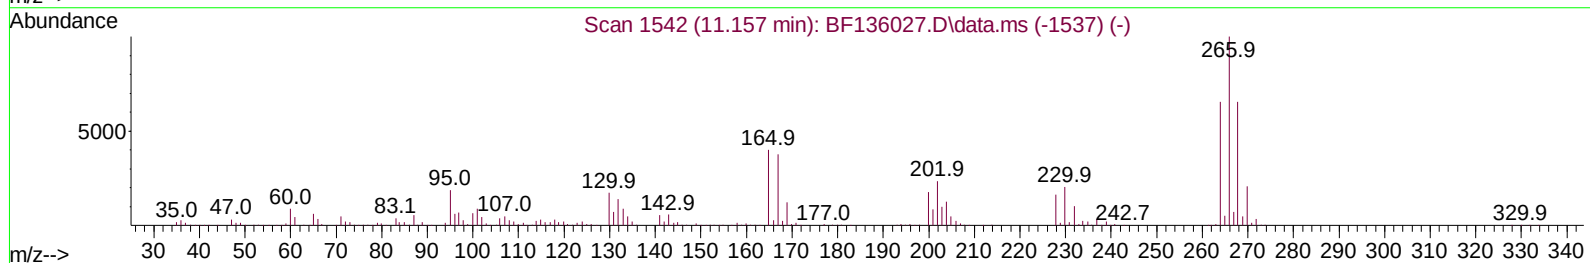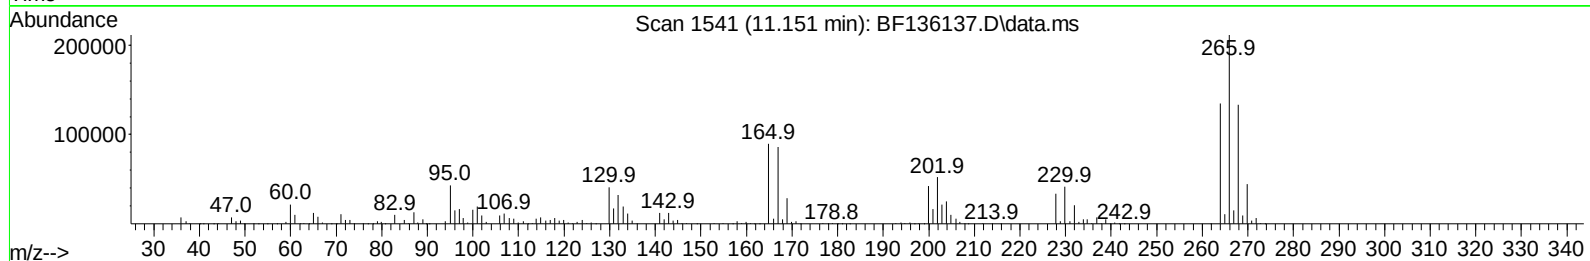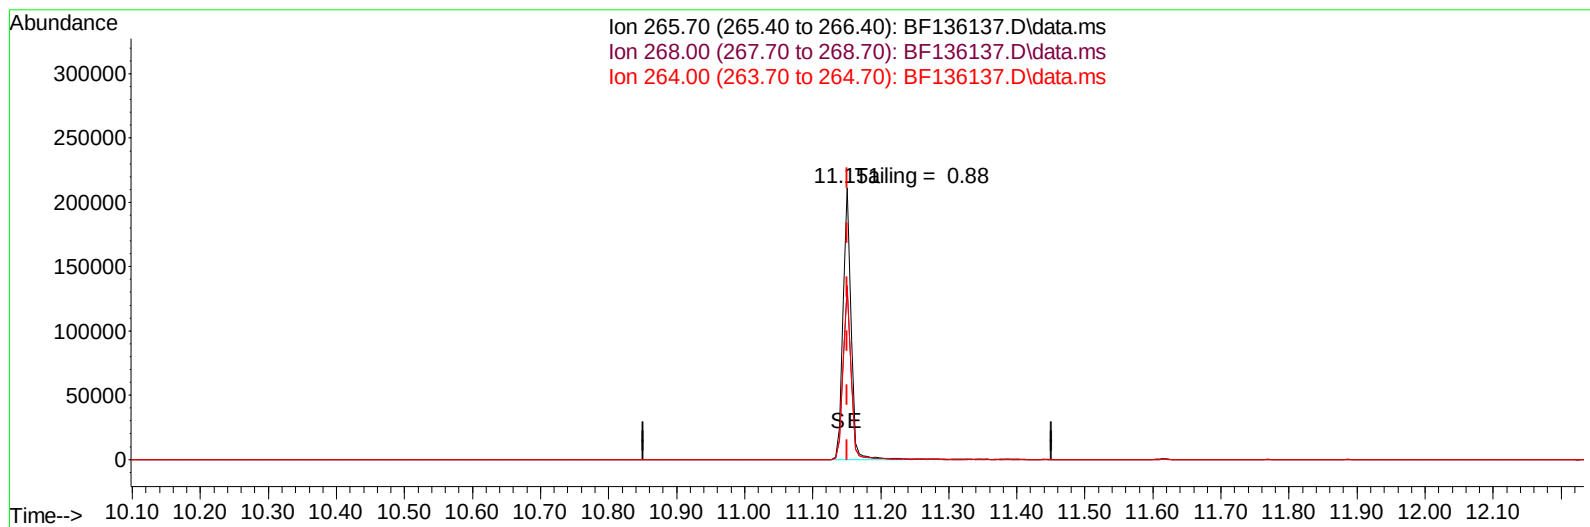

TIC: BF136137.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.000) 283615.11 ng




response 171321

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.18
264.00	65.30	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110423\
Data File : BF136137.D
Acq On : 04 Nov 2023 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 06 01:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 06 00:53:35 2023
Response via : Initial Calibration

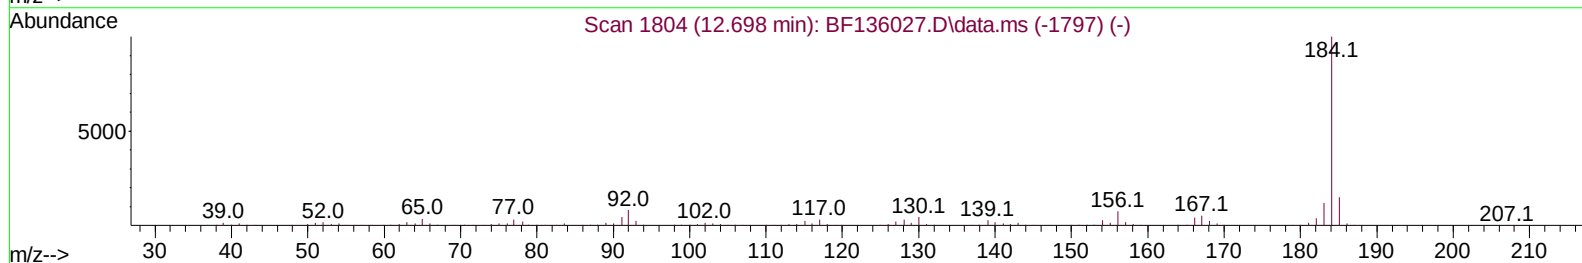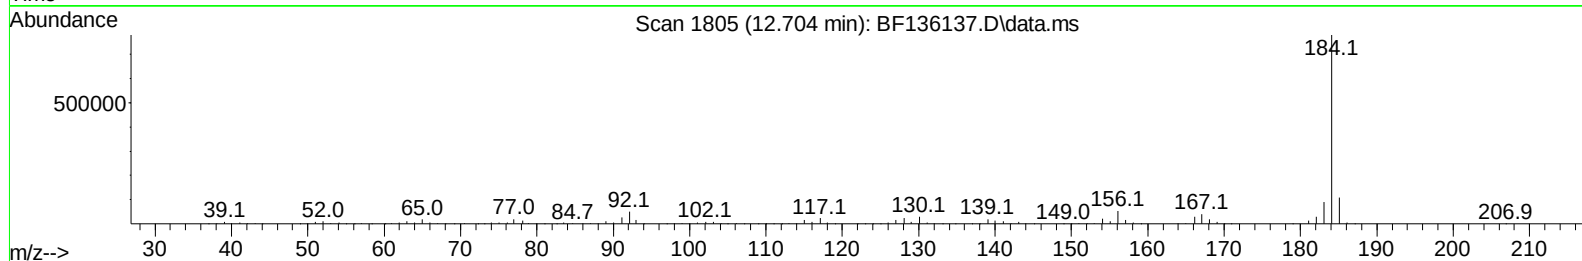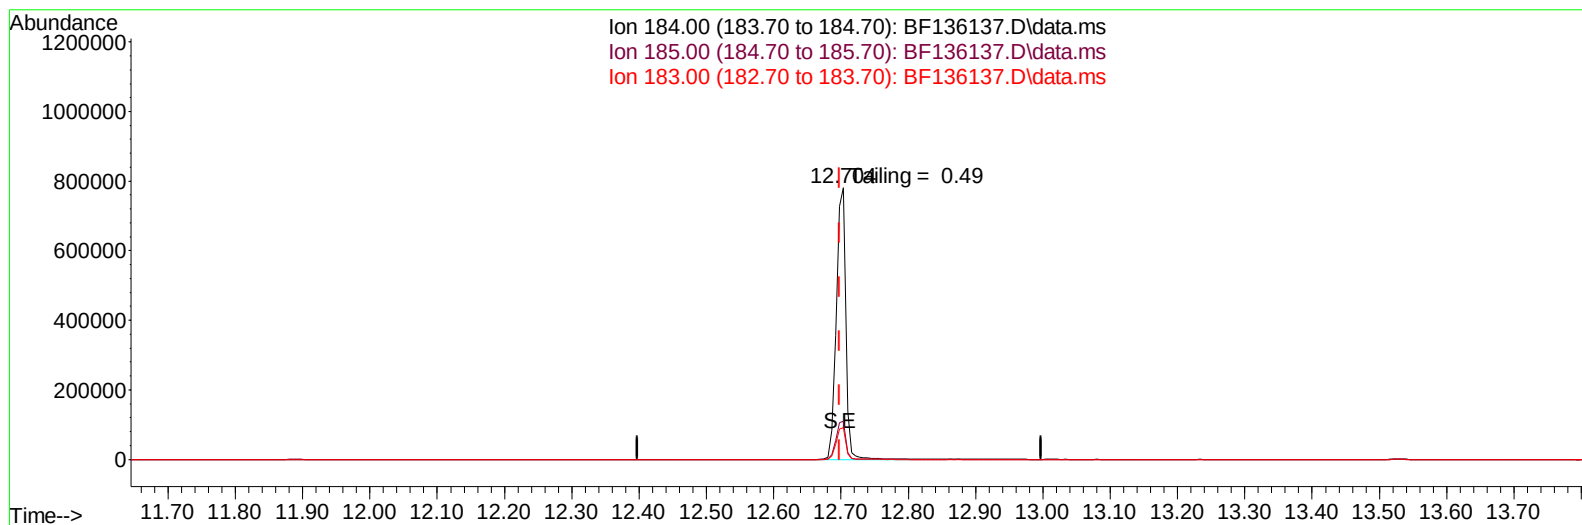

TIC: BF136137.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 285948.45 ng

response 763552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.01
183.00	11.90	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2023	BNA_F	<u>BF136137.D</u>
Compound Name	Response	Retention Time
DDT	382713	13.527
DDD	6433	13.257
DDE	399	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6832	389545	1.75

Instrument :
BNA_F
ClientSampleId :
DFTPP