
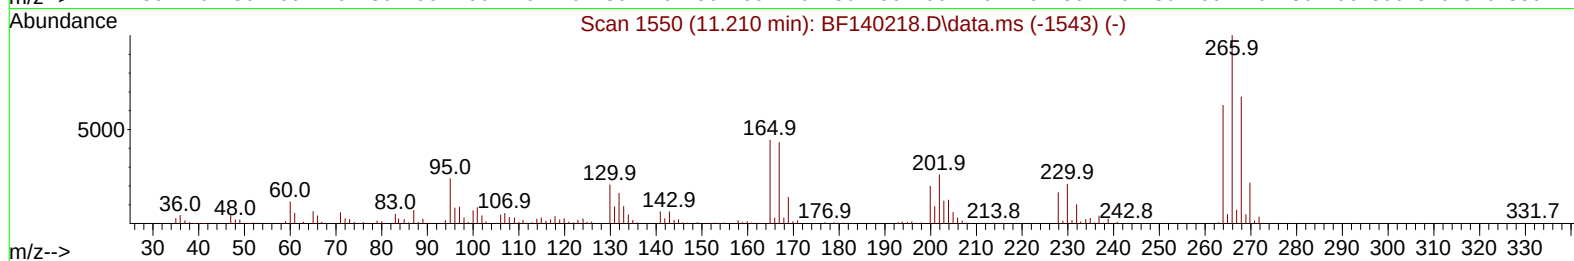
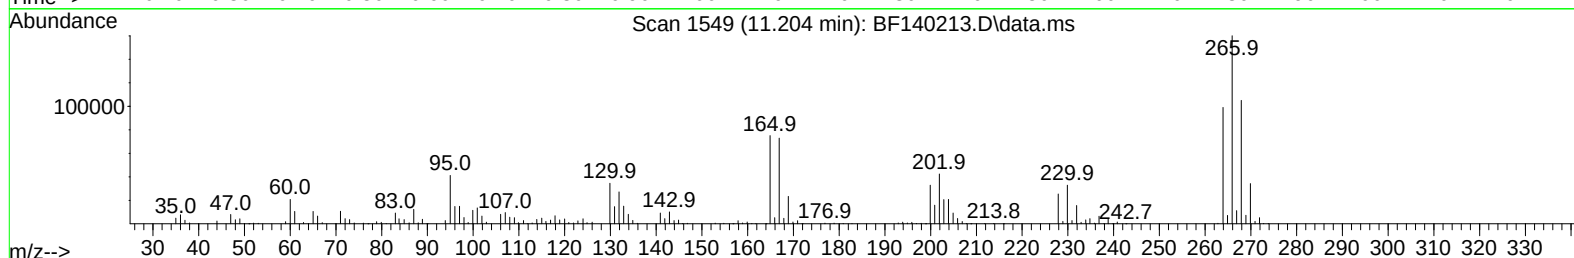


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140213.D
Acq On : 04 Nov 2024 12:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 17:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 16:40:41 2024
Response via : Initial Calibration

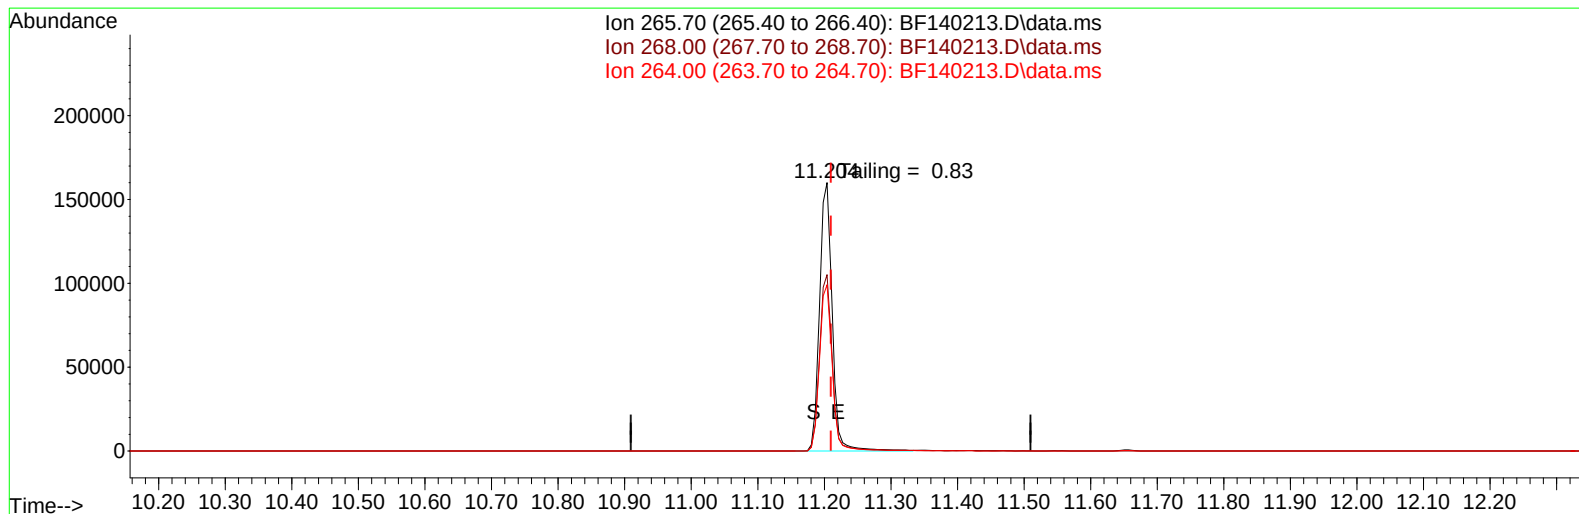

TIC: BF140213.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 130409.06 ng m

response 211836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	65.69
264.00	62.90	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140213.D
Acq On : 04 Nov 2024 12:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 17:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 16:40:41 2024
Response via : Initial Calibration

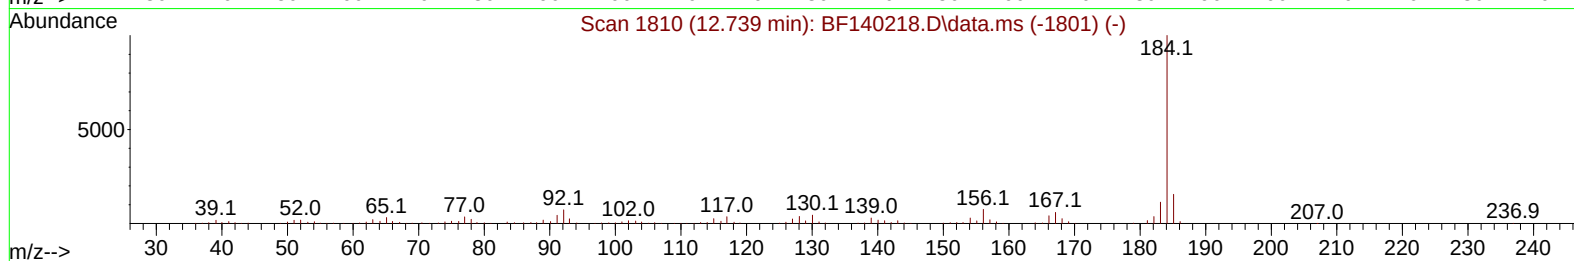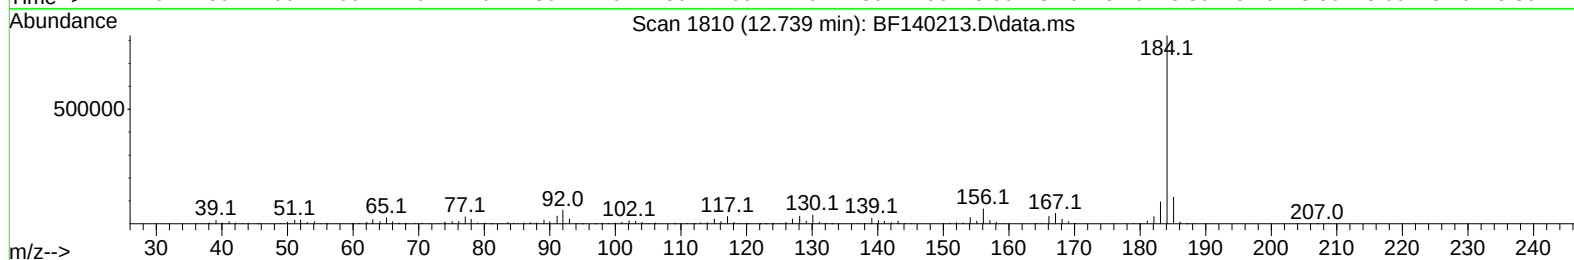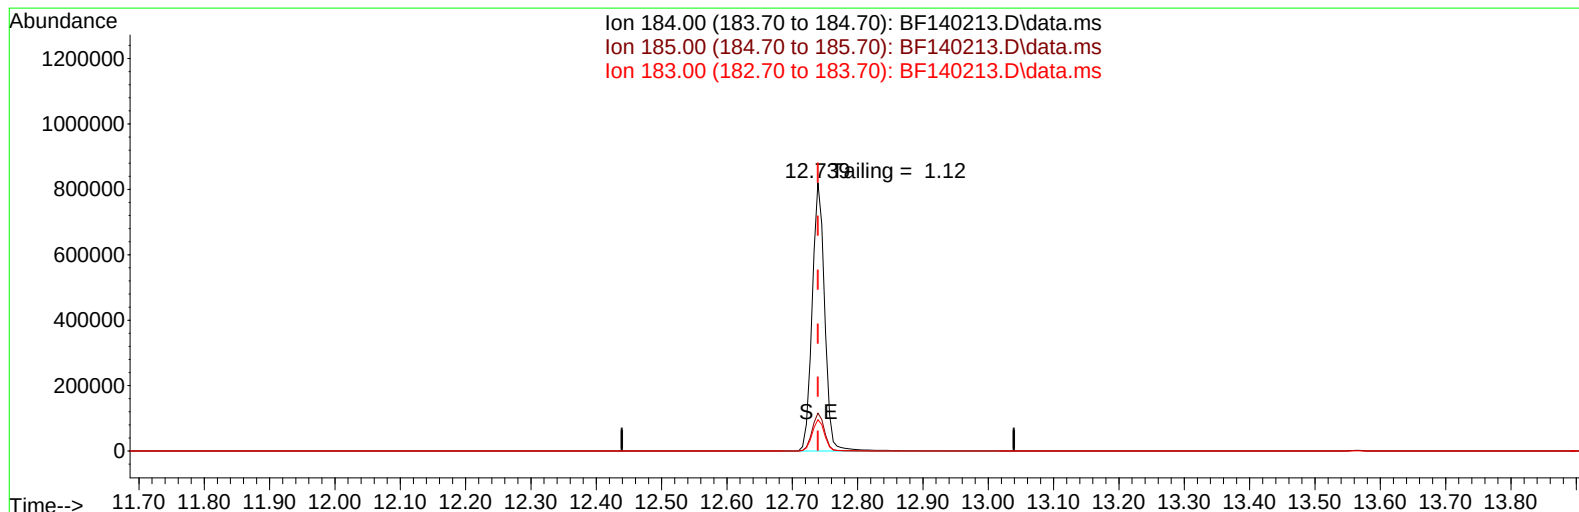

TIC: BF140213.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 270994.89 ng

response 1090575

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	11.30	11.70
0.00	0.00	0.00