

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140223.D
Acq On : 04 Nov 2024 17:23
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	574	581	586	rBV	4504114	6462261	62.16%	11.954%
2	6.504	742	750	755	rBV	4113301	6570677	63.20%	12.155%
3	6.875	808	813	818	rBV	1156593	1407585	13.54%	2.604%
4	7.434	901	908	914	rBV	3006902	4391255	42.24%	8.123%
5	8.151	1024	1030	1036	rBV	1345830	1859734	17.89%	3.440%
6	9.234	1206	1214	1219	rBV	5557710	8861236	85.23%	16.392%
7	9.910	1322	1329	1344	rVB	1646539	2273333	21.87%	4.205%
8	10.704	1455	1464	1496	rBV	4218607	5921097	56.95%	10.953%
9	11.404	1573	1583	1588	rBV	1926513	2461529	23.68%	4.553%
10	12.998	1847	1854	1859	rBV	7527327	10396820	100.00%	19.233%
11	14.051	2024	2033	2043	rBV	1395788	2015457	19.39%	3.728%
12	15.545	2280	2287	2302	rBV	899371	1437108	13.82%	2.658%




Sum of corrected areas: 54058092

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140223.D
Acq On : 04 Nov 2024 17:23
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

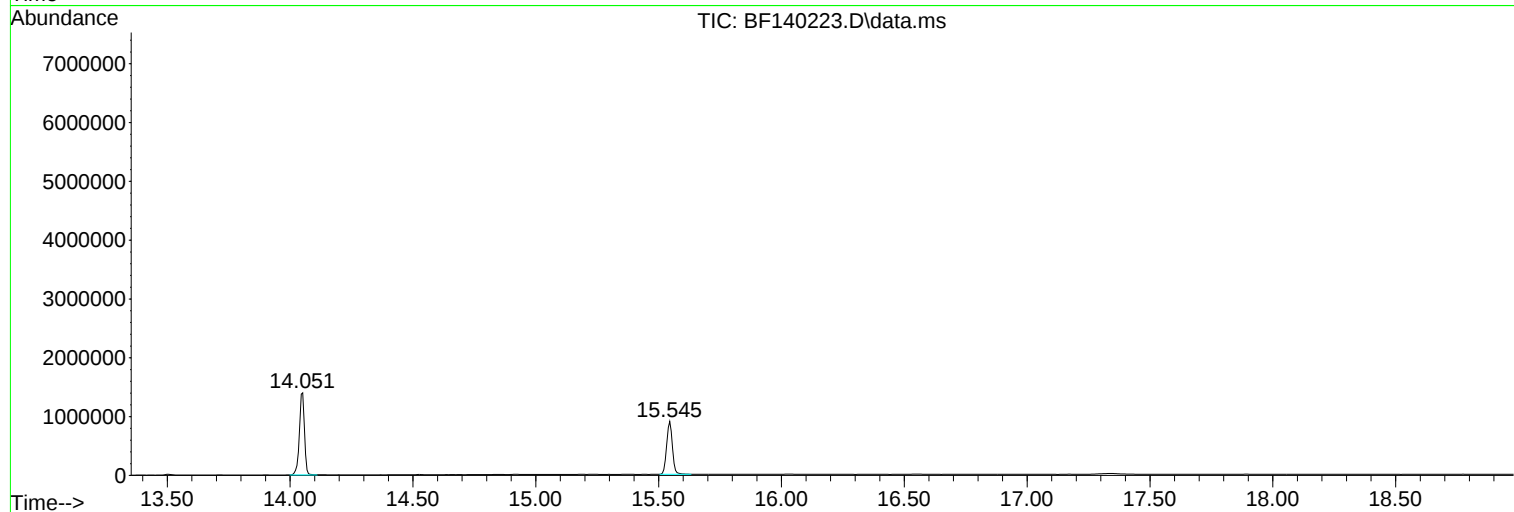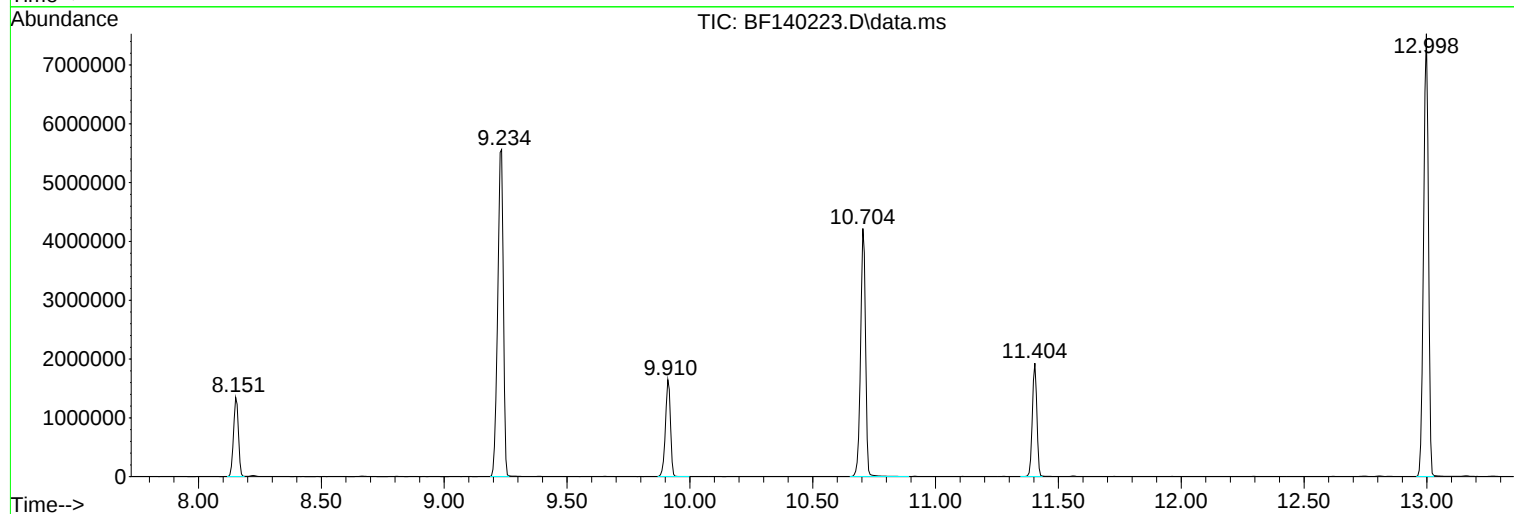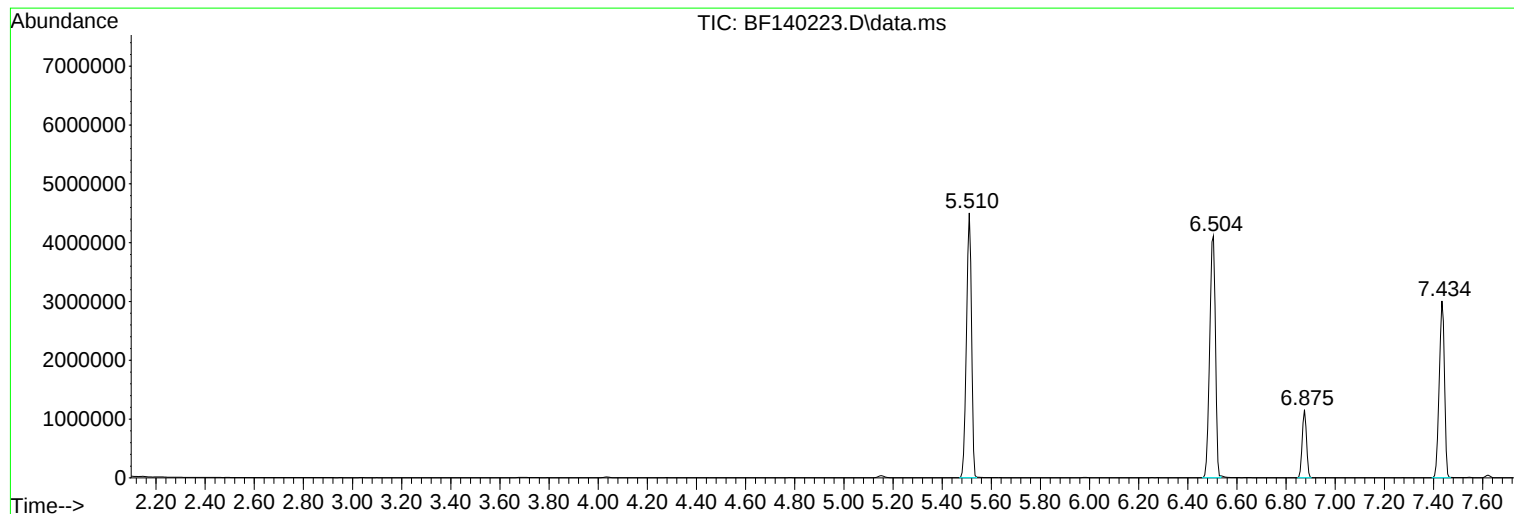

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140223.D
Acq On : 04 Nov 2024 17:23
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140223.D
Acq On : 04 Nov 2024 17:23
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------