

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140228.D
Acq On : 04 Nov 2024 19:33
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164382BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	574	581	586	rBV	4540032	6595093	62.75%	11.977%
2	6.504	742	750	755	rBV	4129563	6714977	63.89%	12.194%
3	6.875	808	813	818	rBV	1188686	1458421	13.88%	2.648%
4	7.434	901	908	914	rBV	3047050	4473029	42.56%	8.123%
5	8.151	1024	1030	1036	rBV	1385274	1907470	18.15%	3.464%
6	9.234	1206	1214	1219	rBV	5732044	9041829	86.03%	16.420%
7	9.910	1322	1329	1335	rBV	1680996	2320621	22.08%	4.214%
8	10.704	1455	1464	1494	rBV	4309395	6010401	57.19%	10.915%
9	11.404	1574	1583	1588	rBV	1950898	2530493	24.08%	4.595%
10	12.998	1847	1854	1859	rBV	7419380	10510309	100.00%	19.087%
11	14.045	2024	2032	2042	rBV	1507279	2045354	19.46%	3.714%
12	15.533	2278	2285	2304	rBV	915200	1458557	13.88%	2.649%




Sum of corrected areas: 55066554

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140228.D
Acq On : 04 Nov 2024 19:33
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

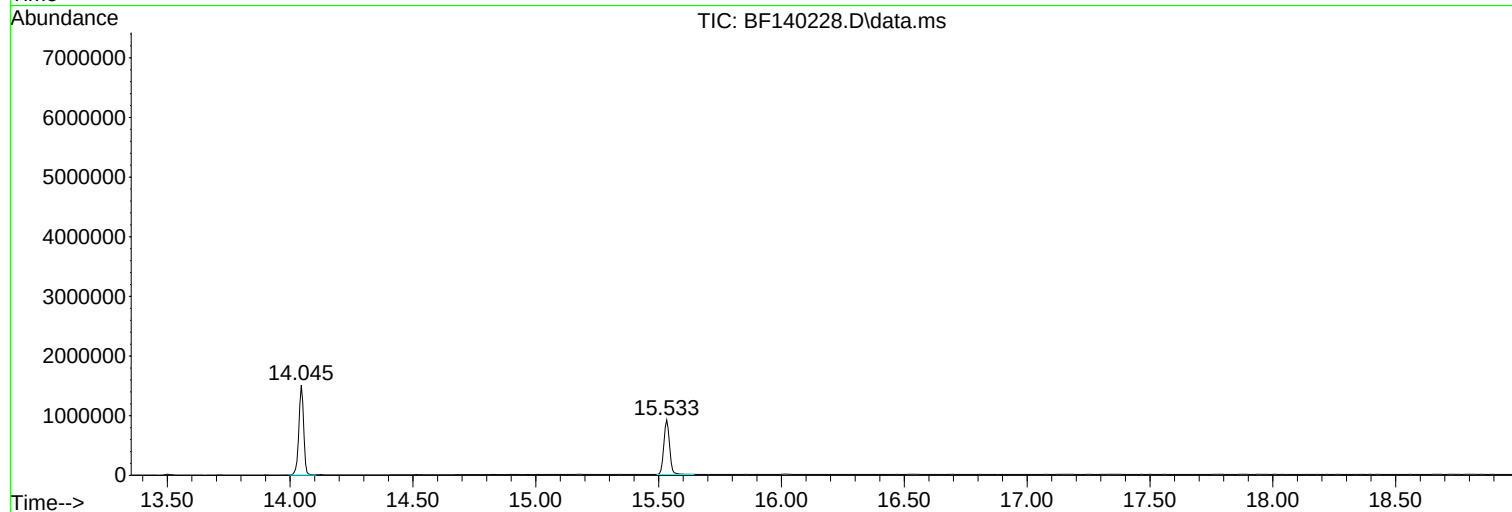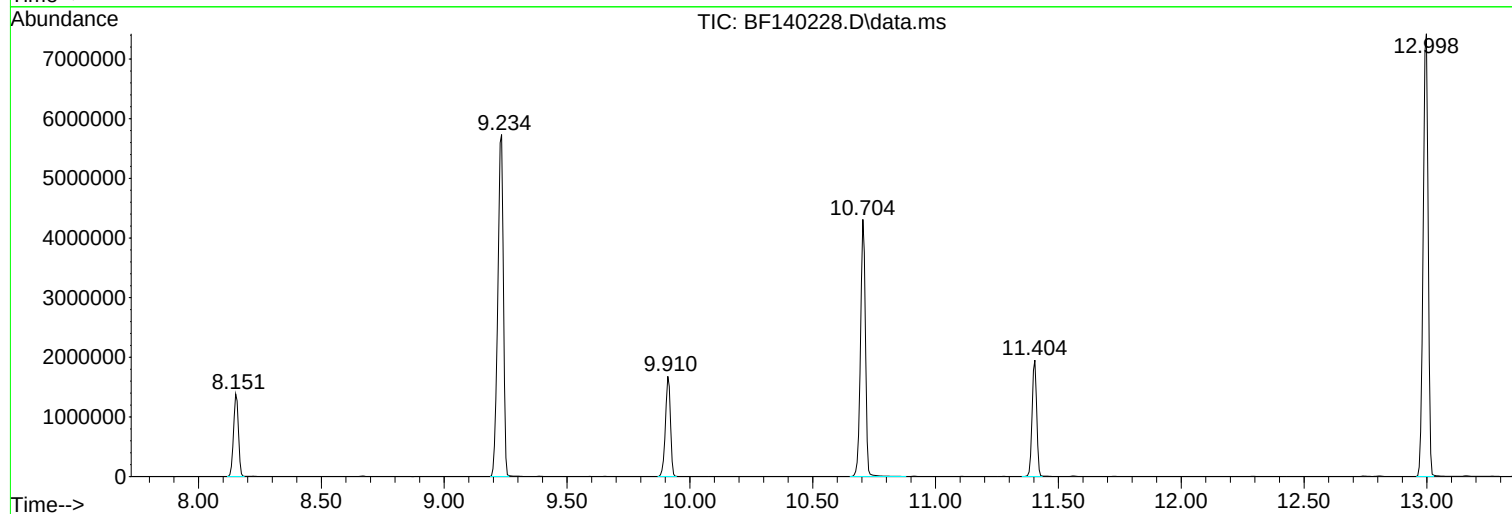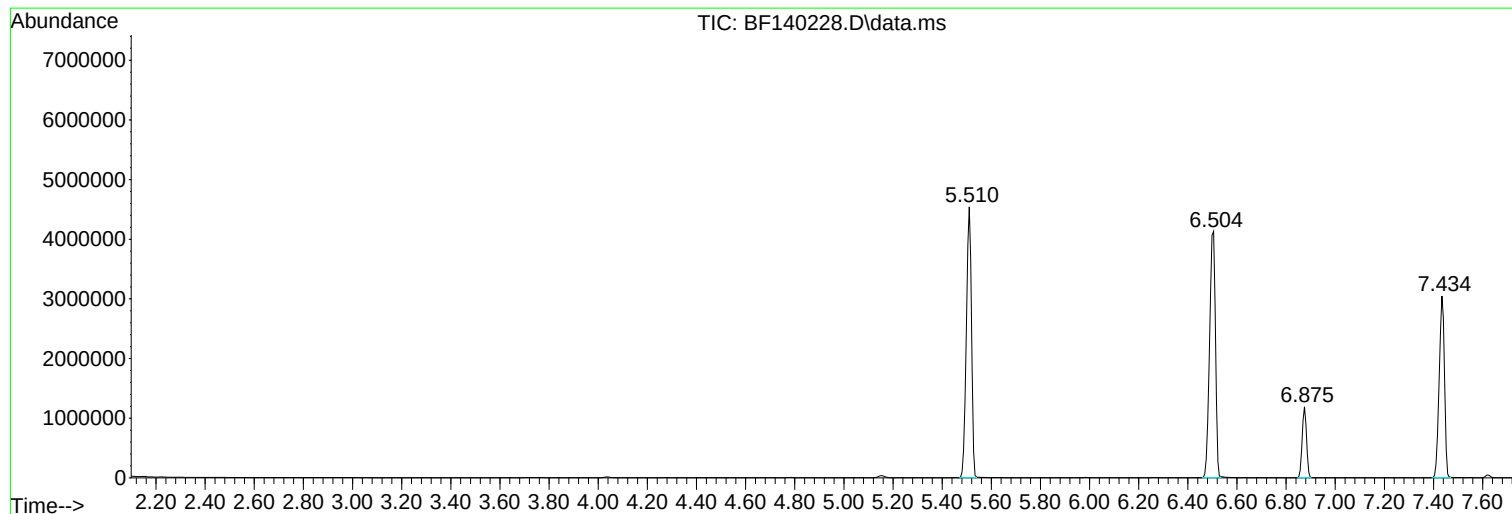

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140228.D
Acq On : 04 Nov 2024 19:33
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140228.D
Acq On : 04 Nov 2024 19:33
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------