


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140213.D
Acq On : 04 Nov 2024 12:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 04 17:12:57 2024

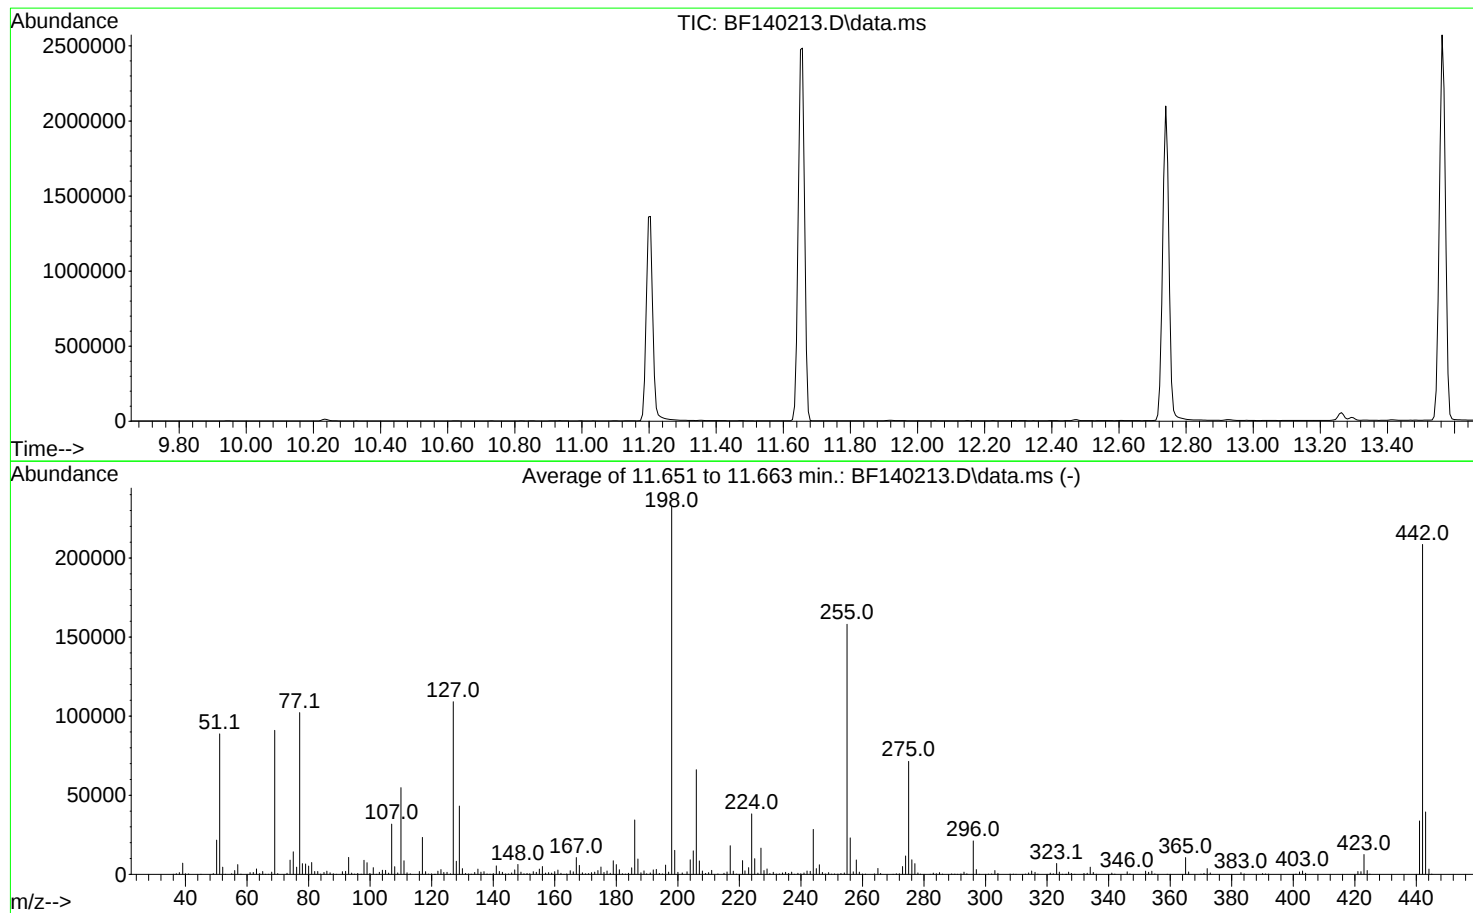




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	88763	PASS
68	69	0.00	2	1.6	1436	PASS
69	198	0.00	100	39.2	91045	PASS
70	69	0.00	2	0.6	512	PASS
127	198	10	80	46.9	109144	PASS
197	198	0.00	2	0.6	1408	PASS
198	198	100	100	100.0	232533	PASS
199	198	5	9	6.5	15148	PASS
275	198	10	60	30.7	71416	PASS
365	198	1	100	4.6	10598	PASS
441	198	0.01	100	14.5	33741	PASS
442	442	50	100	100.0	208555	PASS
443	442	15	24	18.9	39440	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140213.D
Acq On : 04 Nov 2024 12:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 17:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 16:40:41 2024
Response via : Initial Calibration

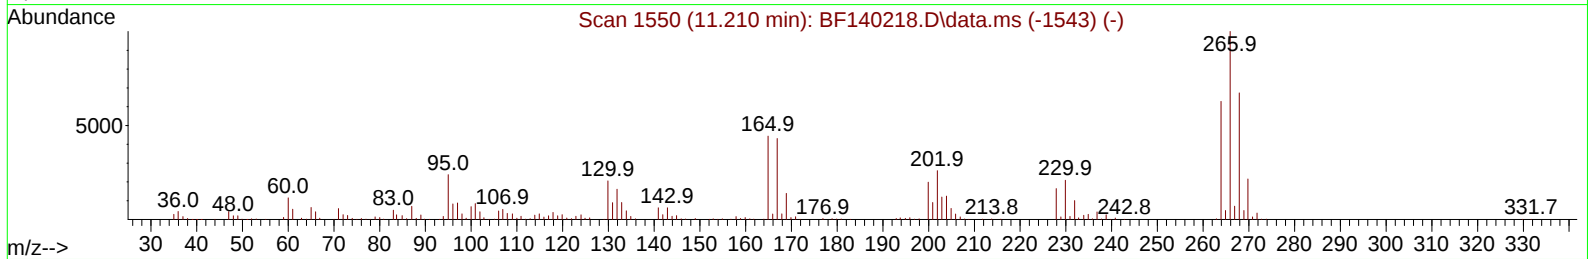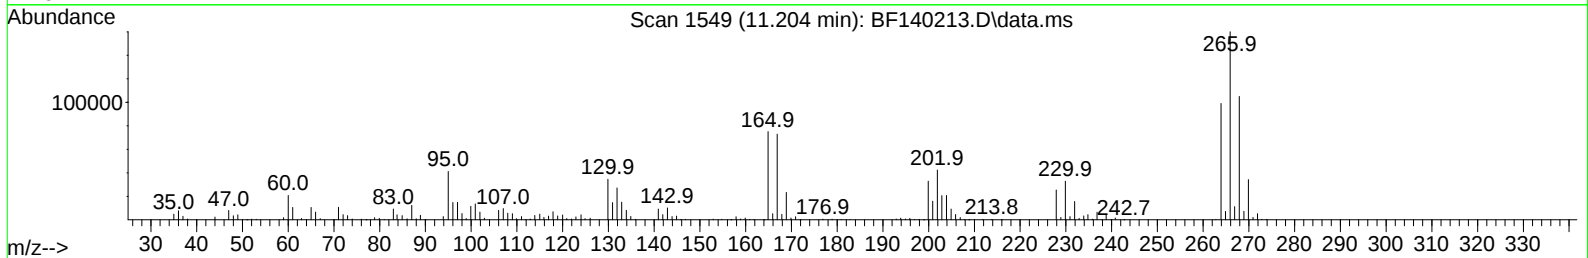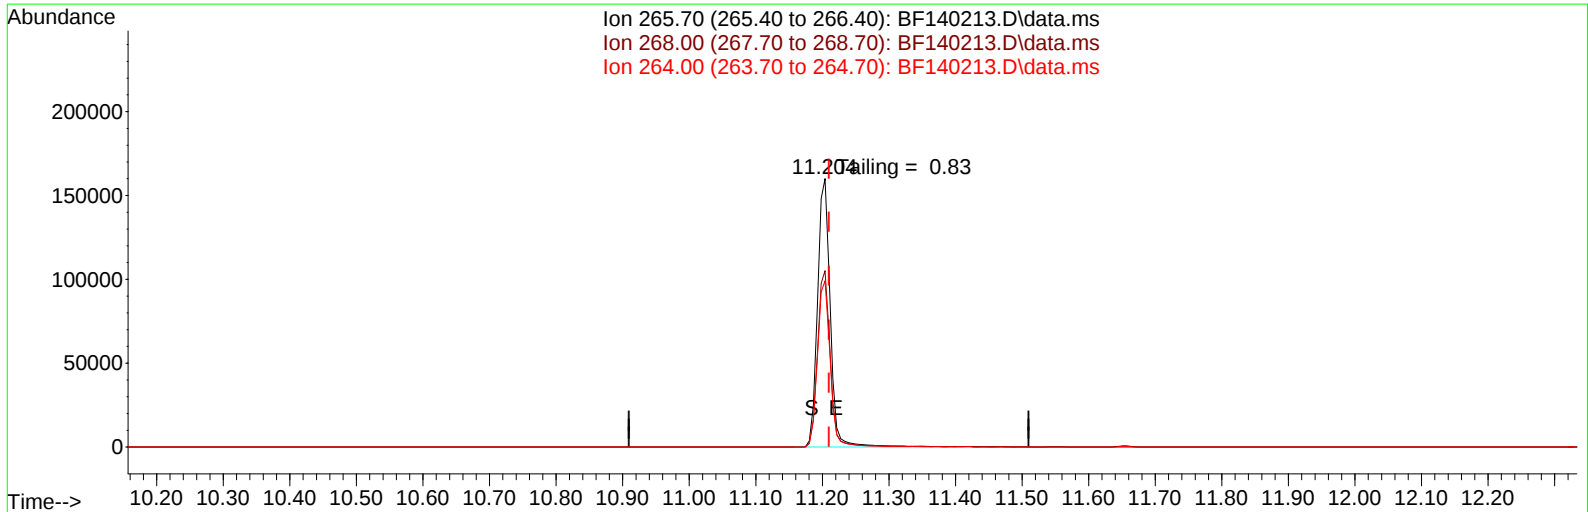

TIC: BF140213.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 130409.06 ng m




response 211836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	65.69
264.00	62.90	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110424\
Data File : BF140213.D
Acq On : 04 Nov 2024 12:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 04 17:09:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 16:40:41 2024
Response via : Initial Calibration

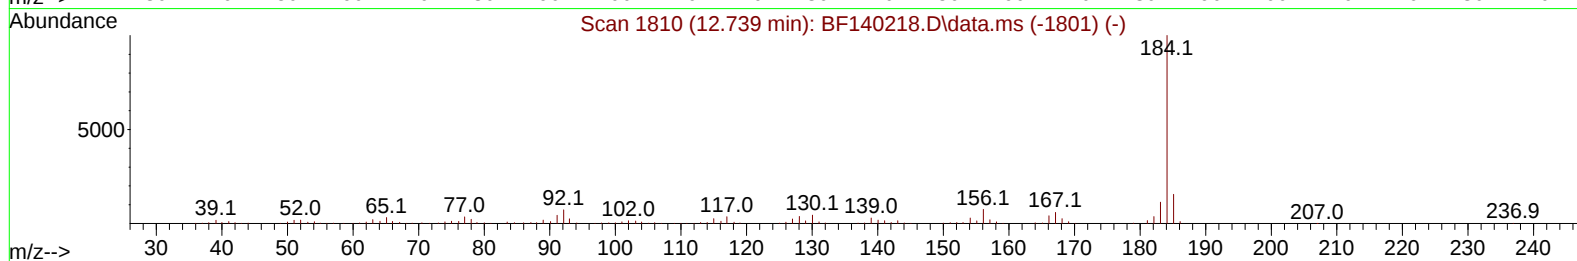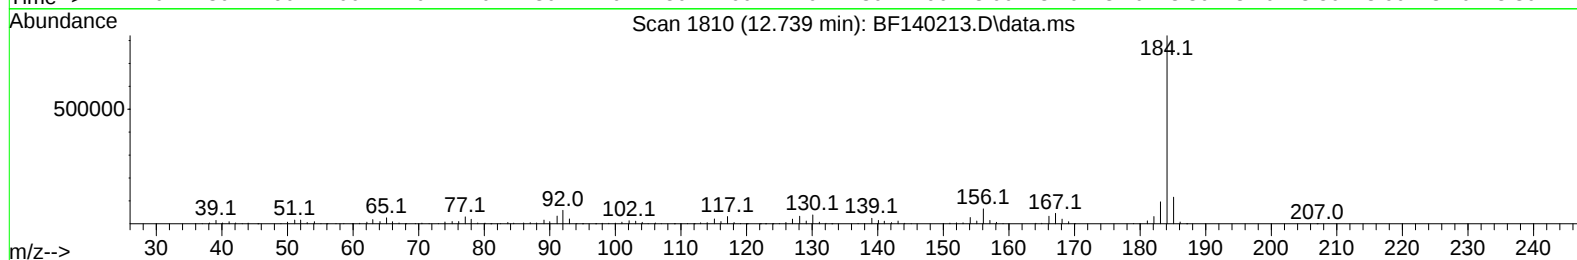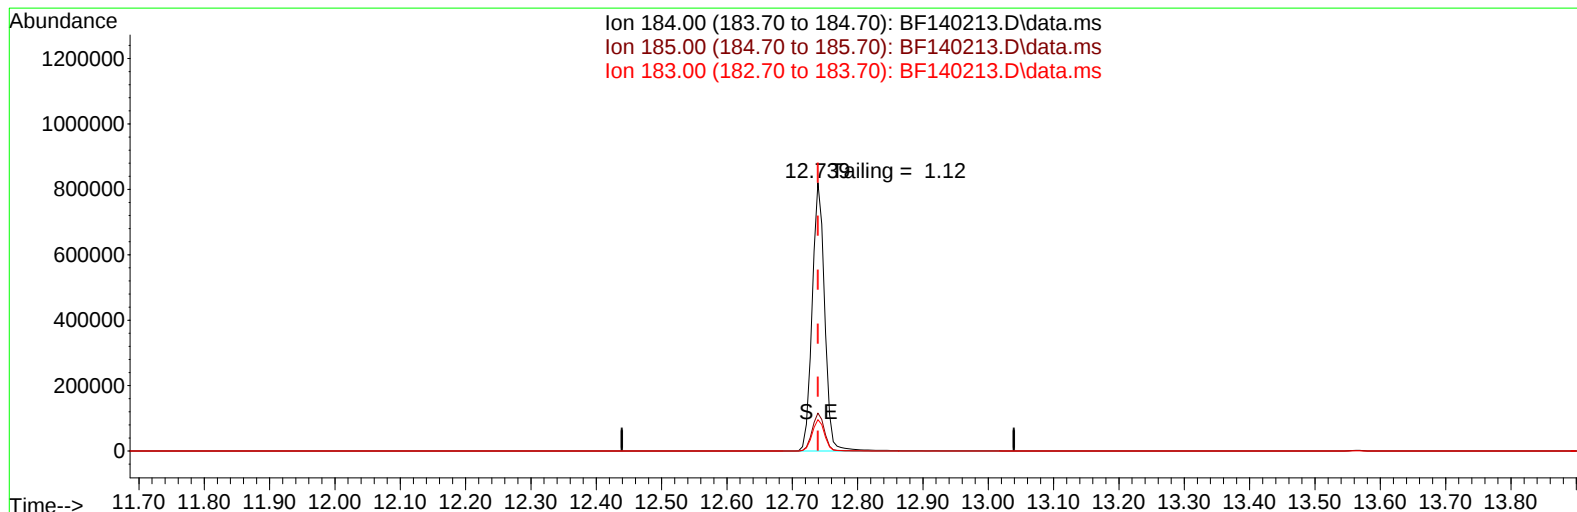

TIC: BF140213.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 270994.89 ng

response 1090575

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.13
183.00	11.30	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2024	BNA_F	<u>BF140213.D</u>
Compound Name	Response	Retention Time
DDT	588456	13.563
DDD	17211	13.263
DDE	1858	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19069	607525	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP