
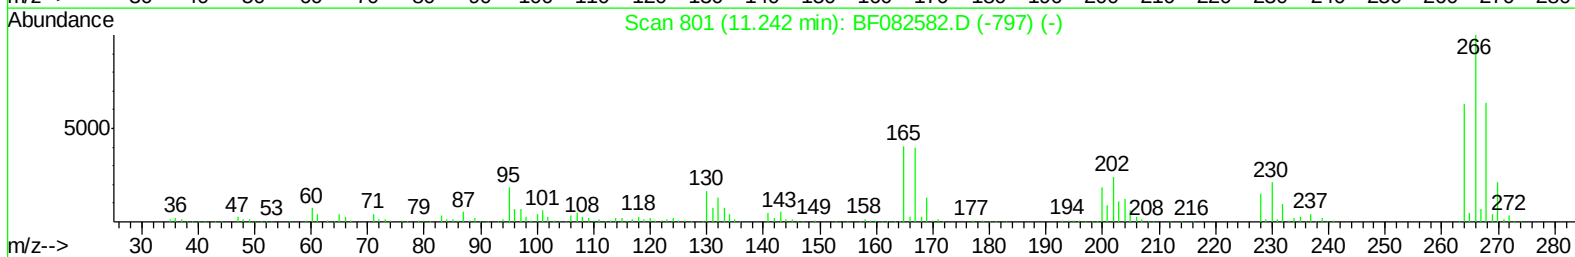
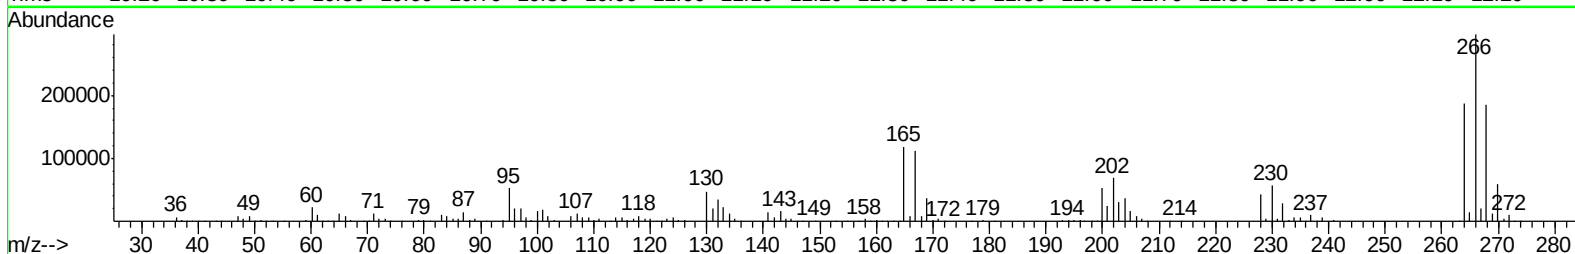


Data Path : Z:\HPCHEM1\BNA_F\Data\BF110515\
Data File : BF082694.D
Acq On : 4 Nov 2015 11:57
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 07:46:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

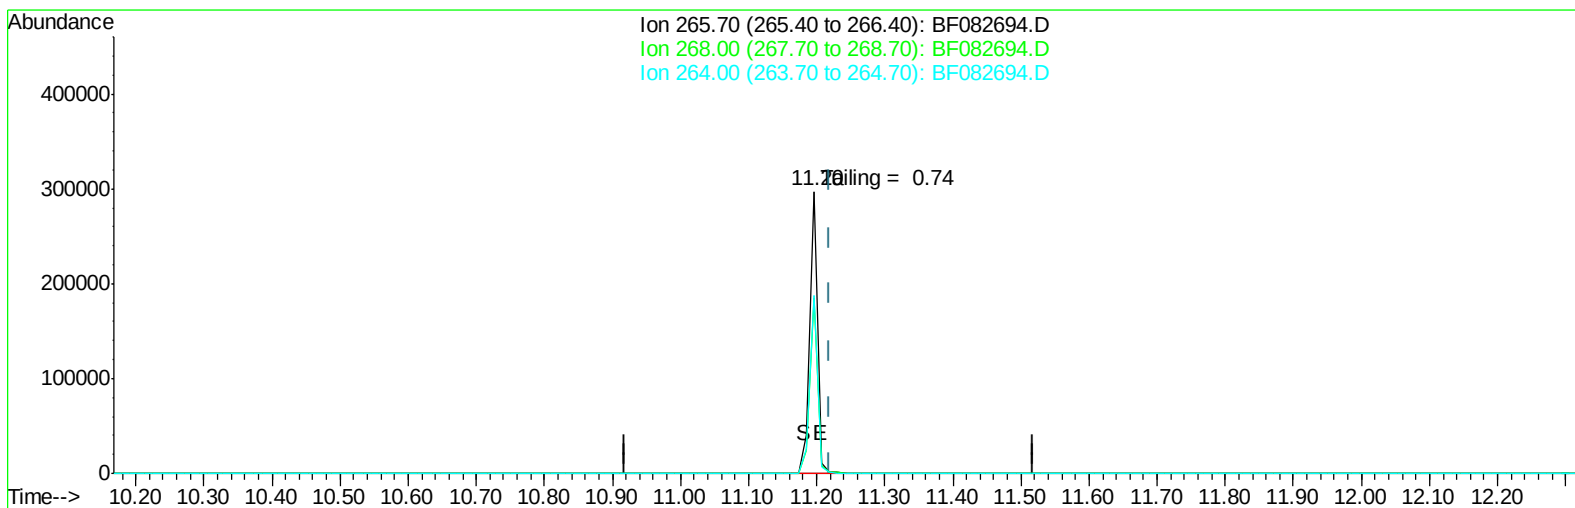

TIC: BF082694.D

(69) Pentachlorophenol (C)




11.196min (-0.023) 0.00ng

response 243085

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.38
264.00	63.20	63.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF110515\
Data File : BF082694.D
Acq On : 4 Nov 2015 11:57
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 07:46:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

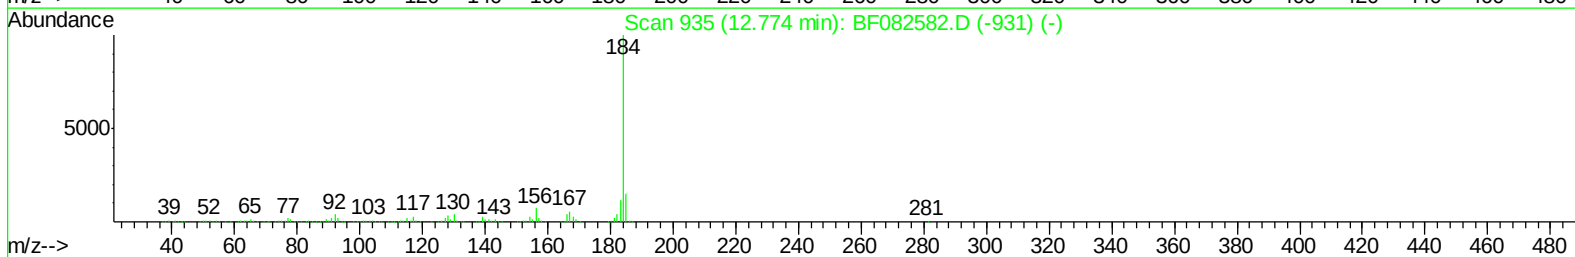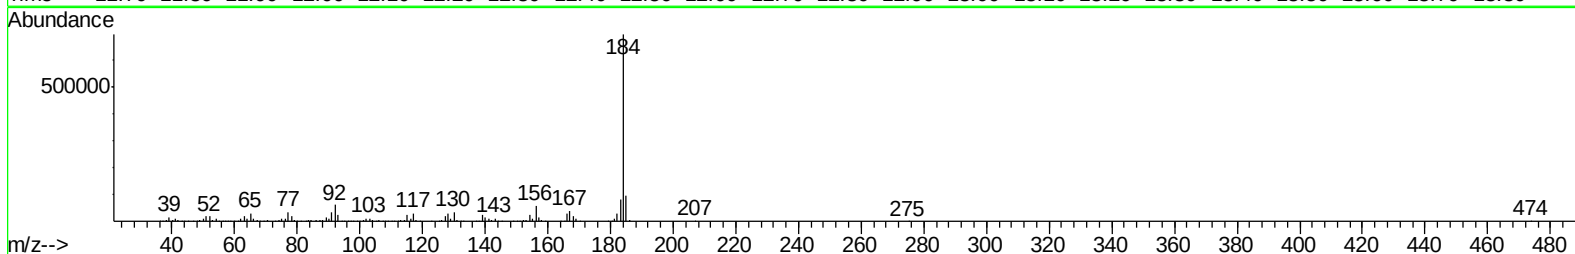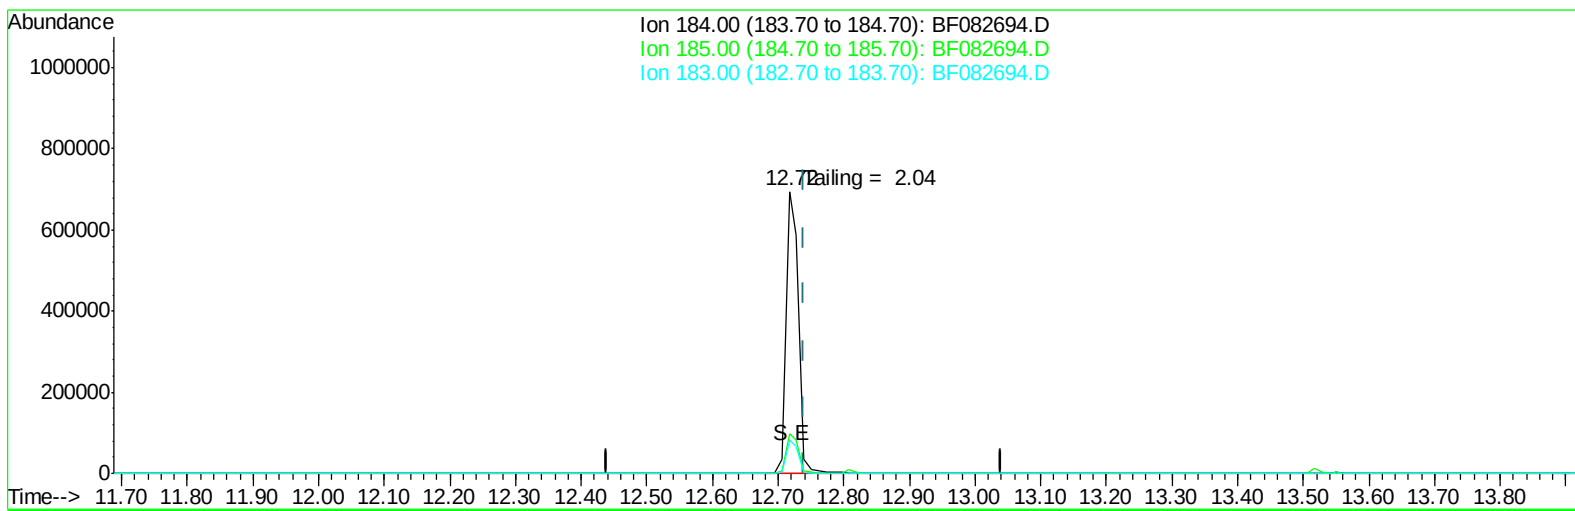

TIC: BF082694.D

(76) Benzidine

12.717min (-0.023) 28853.44ng

response 947320

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.08
183.00	12.00	12.04
0.00	0.00	0.00