

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110515\
 Data File : BF082704.D
 Acq On : 4 Nov 2015 16:47
 Operator : UM/IZ
 Sample : G4240-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-05(18-20)

Quant Time: Nov 05 05:41:52 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 03 12:27:47 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	191949	20.00	ng	-0.01
21) Naphthalene-d8	8.14	136	674917	20.00	ng	-0.02
38) Acenaphthene-d10	9.90	164	402067	20.00	ng	-0.02
63) Phenanthrene-d10	11.39	188	714227	20.00	ng	-0.02
75) Chrysene-d12	14.03	240	693293	20.00	ng	-0.02
86) Perylene-d12	15.48	264	527046	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	1615931	126.80	ng	0.01
7) Phenol-d6	6.50	99	1842101	108.80	ng	-0.01
23) Nitrobenzene-d5	7.42	82	1266379	76.62	ng	-0.02
41) 2,4,6-Tribromophenol	10.69	330	554245	125.96	ng	-0.02
44) 2-Fluorobiphenyl	9.23	172	2060075	72.75	ng	-0.02
78) Terphenyl-d14	12.98	244	2151180	67.90	ng	-0.02
Target Compounds						
49) Dimethylphthalate	9.62	163	562257	17.12	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110515\
Data File : BF082704.D
Acq On : 4 Nov 2015 16:47
Operator : UM/IZ
Sample : G4240-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-05(18-20)

Quant Time: Nov 05 05:41:52 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

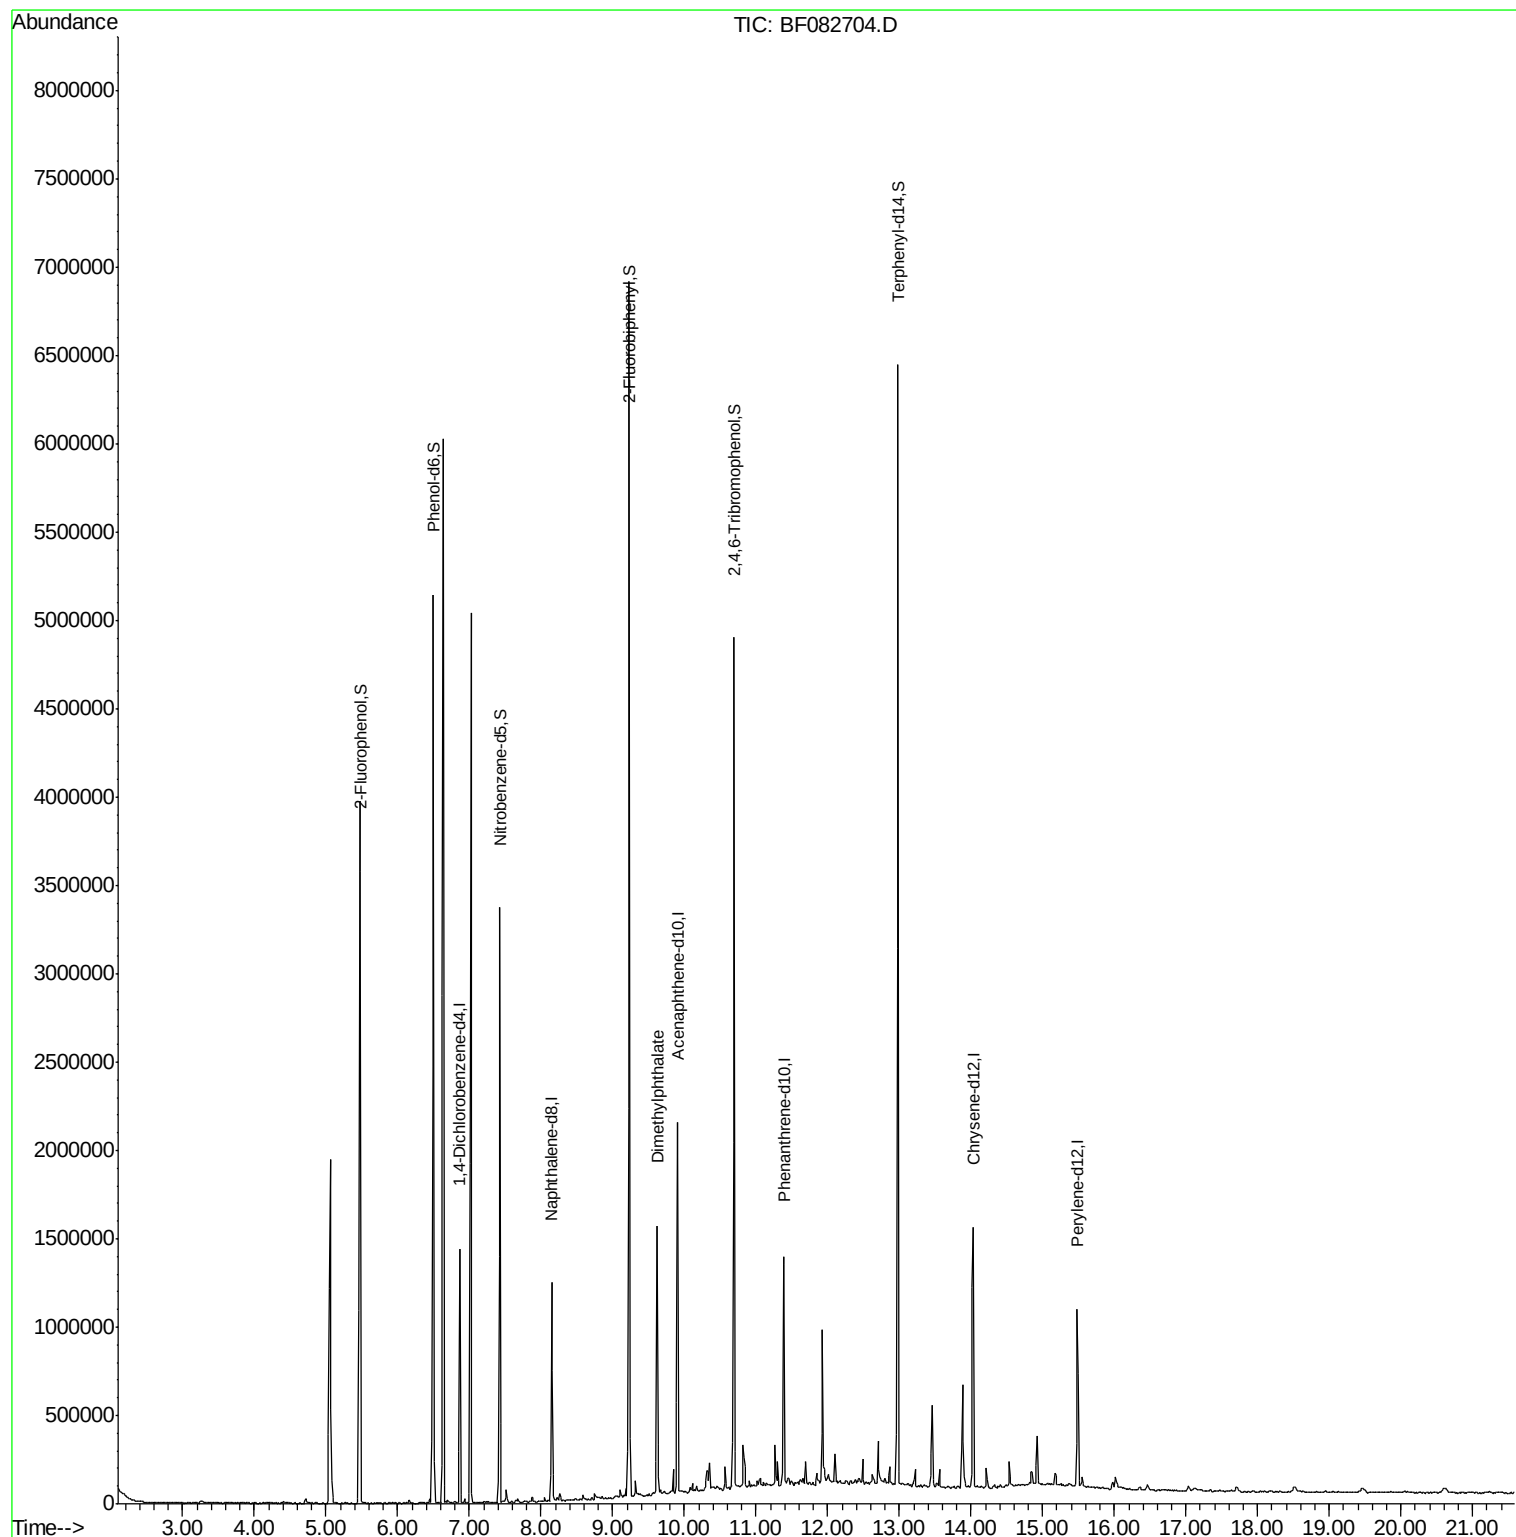




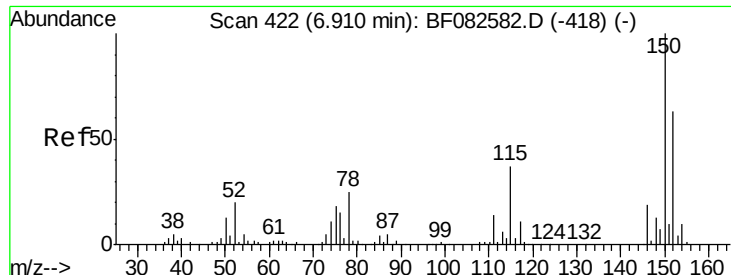


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.86 min Scan# 418
Delta R.T. -0.01 min
Lab File: BF082704.D
Acq: 4 Nov 2015 16:47

Instrument :
BNA_F
ClientSampleId :
SB-05(18-20)




Tot Ion:152 Resp: 191949
Ion Ratio Lower Upper
152 100
150 157.5 127.0 190.4
115 63.5 47.0 70.6

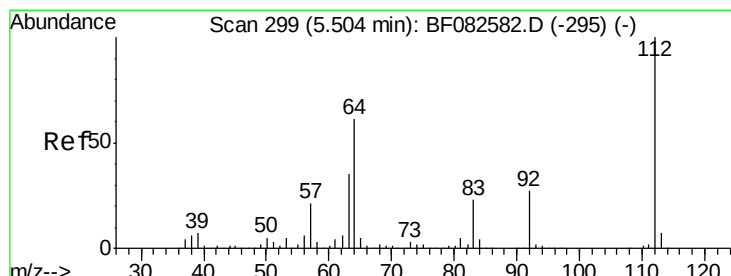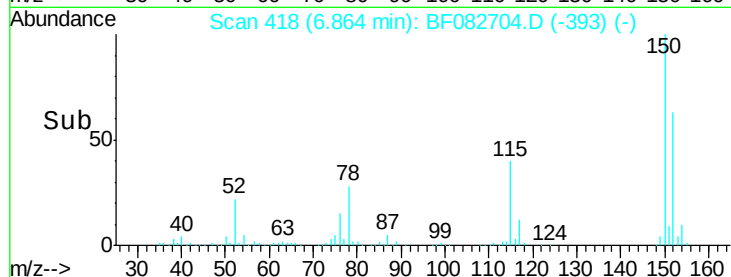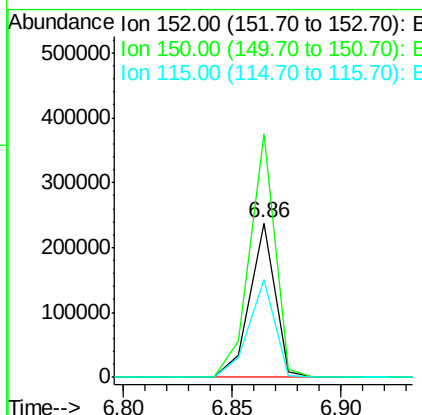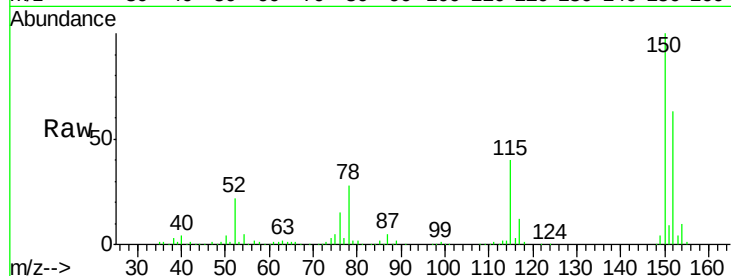


#5

2-Fluorophenol
Concen: 126.80 ng
RT: 5.48 min Scan# 297
Delta R.T. 0.01 min
Lab File: BF082704.D
Acq: 4 Nov 2015 16:47

Tgt Ion:112 Resp: 1615931
Ion Ratio Lower Upper
112 100
64 52.0 48.9 73.3
63 27.8 28.1 42.1#

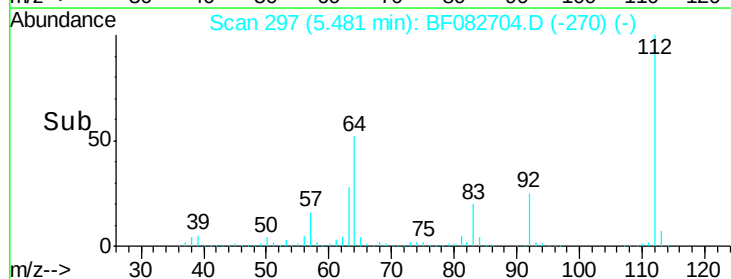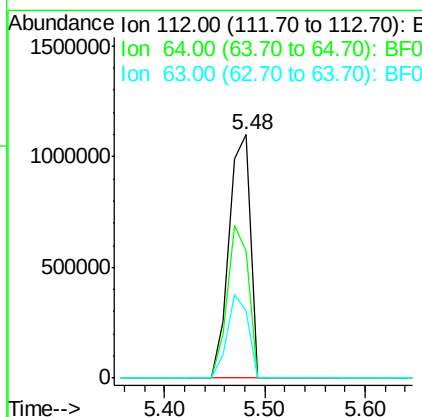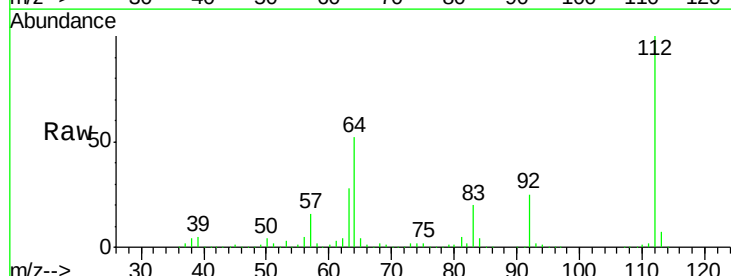

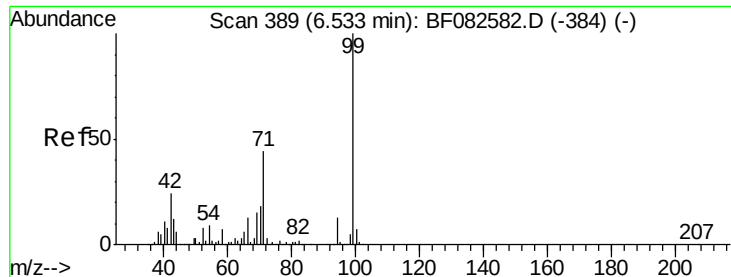

#7

Phenol-d6

Concen: 108.80 ng

RT: 6.50 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47

Instrument :

BNA_F

ClientSampleId :

SB-05(18-20)


Tot Ion: 99 Resp: 1842101

Ion Ratio Lower Upper




99 100

42 22.3 19.2 28.8

71 41.6 35.0 52.4

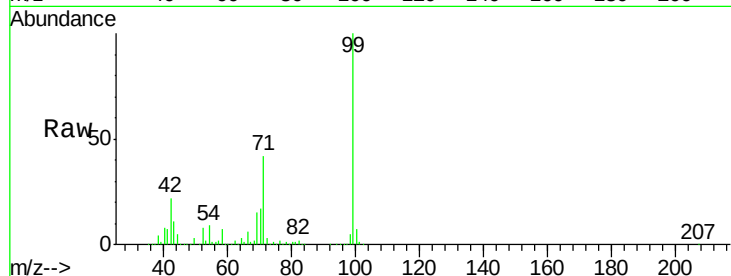

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

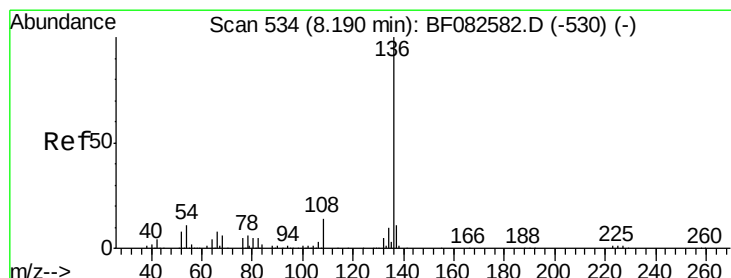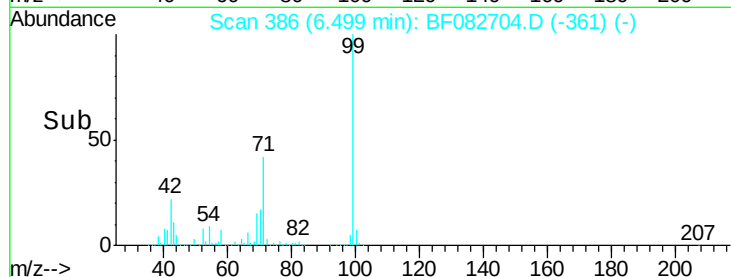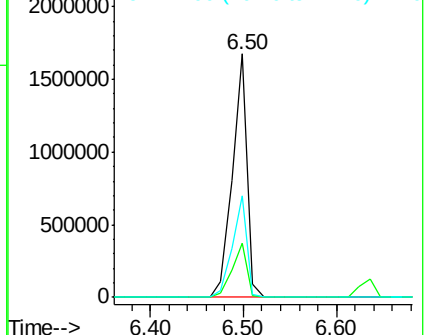

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 530

Delta R.T. -0.02 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47

Tgt Ion: 136 Resp: 674917


Ion Ratio Lower Upper

136 100



137 11.1 9.1 13.7


54 10.9 9.1 13.7

68 6.3 4.8 7.2

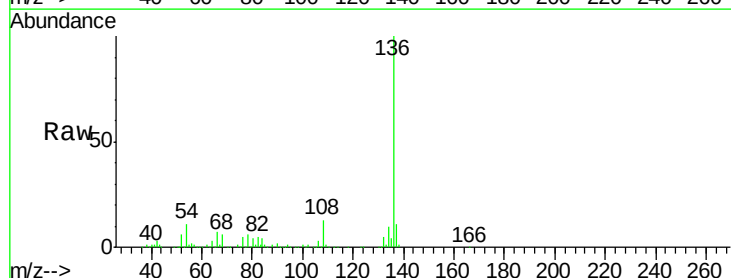

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

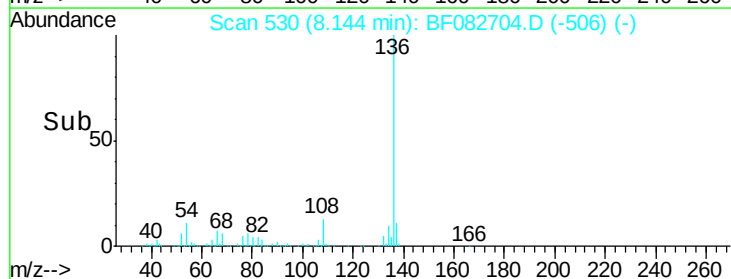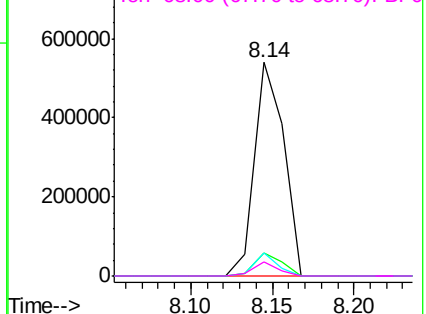


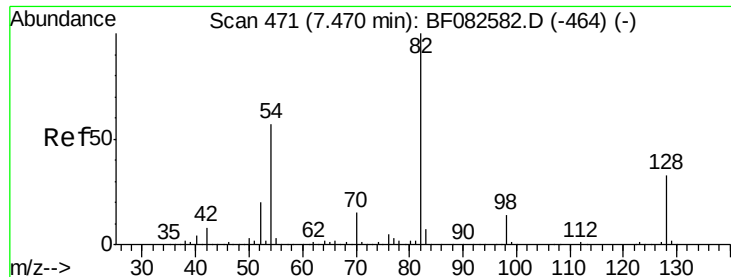




#23
Nitrobenzene-d5
Concen: 76.62 ng
RT: 7.42 min Scan# 467
Delta R.T. -0.02 min
Lab File: BF082704.D
Acq: 4 Nov 2015 16:47

Instrument :
BNA_F
ClientSampleId :
SB-05(18-20)

Tot Ion: 82 Resp: 1266379
Ion Ratio Lower Upper
82 100
128 36.2 26.8 40.2
54 54.5 45.7 68.5

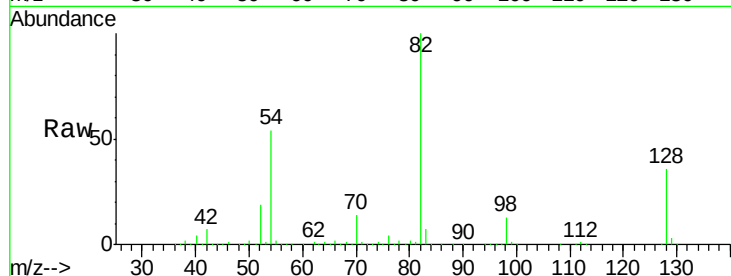


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

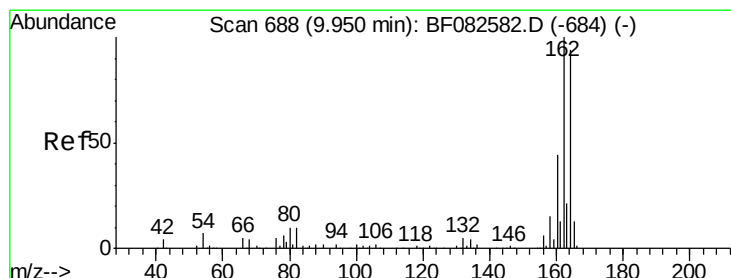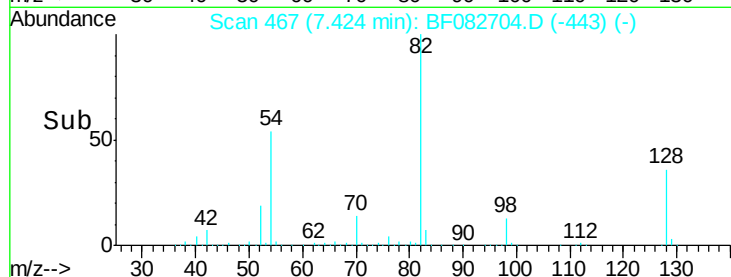
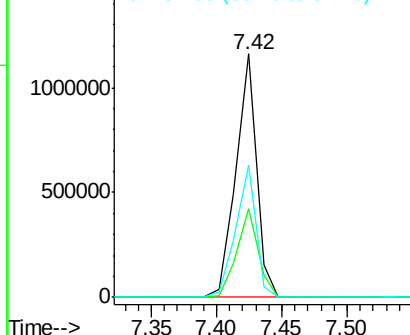



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.90 min Scan# 684
Delta R.T. -0.02 min
Lab File: BF082704.D
Acq: 4 Nov 2015 16:47

Tgt Ion:164 Resp: 402067
Ion Ratio Lower Upper
164 100
162 102.1 84.9 127.3
160 46.6 37.5 56.3

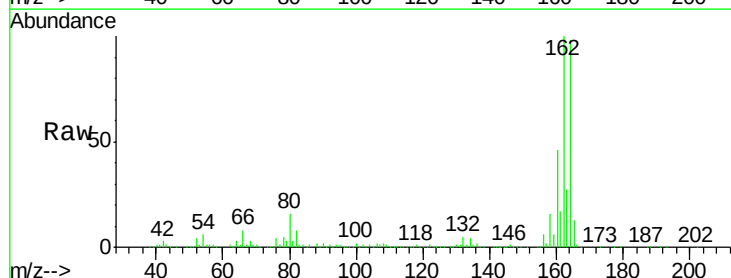

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

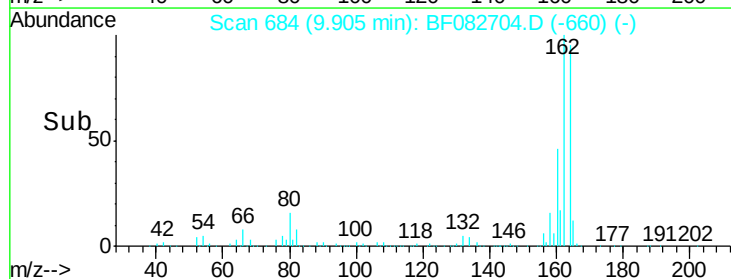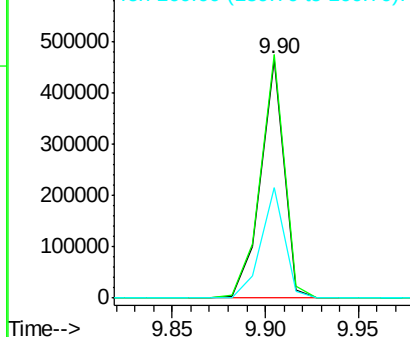


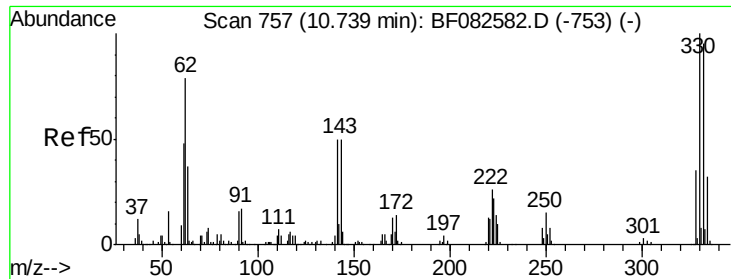




#41
 2,4,6-Tribromophenol
 Concen: 125.96 ng
 RT: 10.69 min Scan# 753
 Delta R.T. -0.02 min
 Lab File: BF082704.D
 Acq: 4 Nov 2015 16:47

Instrument :
 BNA_F
 ClientSampleId :
 SB-05(18-20)

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.1	76.6	114.8
141	42.7	41.2	61.8

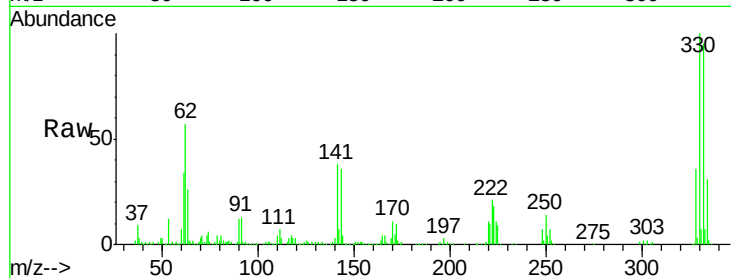


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

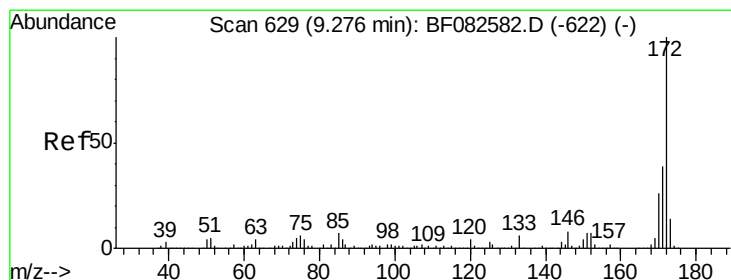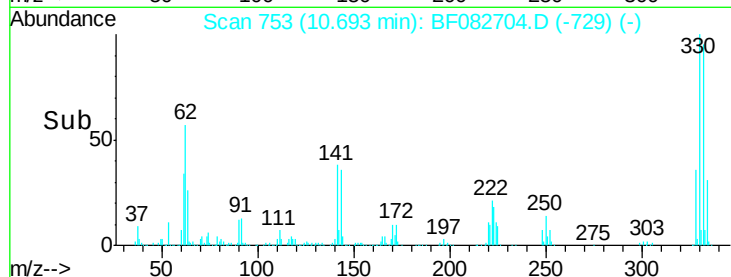
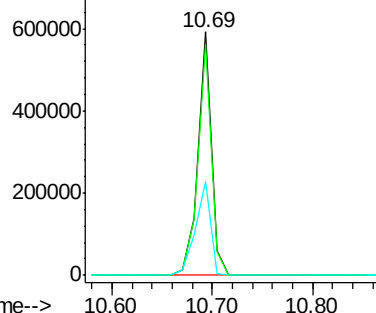



#44
 2-Fluorobiphenyl
 Concen: 72.75 ng
 RT: 9.23 min Scan# 625
 Delta R.T. -0.02 min
 Lab File: BF082704.D
 Acq: 4 Nov 2015 16:47

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.4	30.8	46.2
170	25.7	21.2	31.8

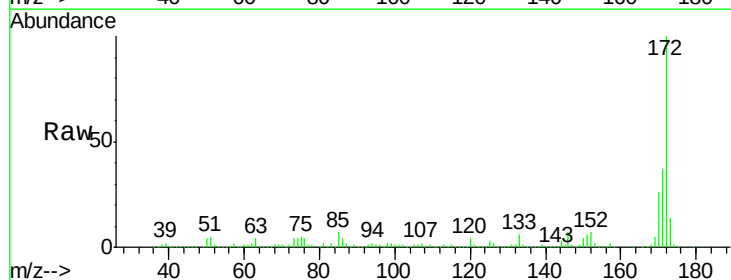

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

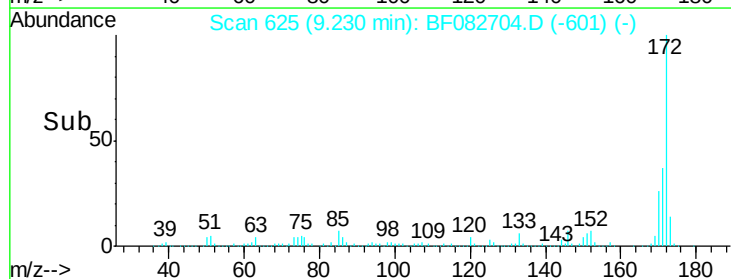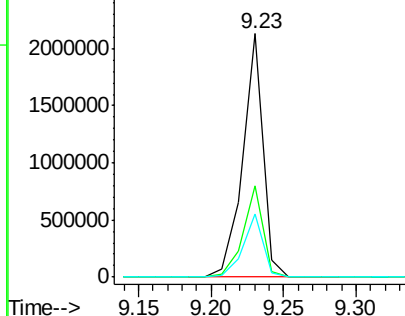

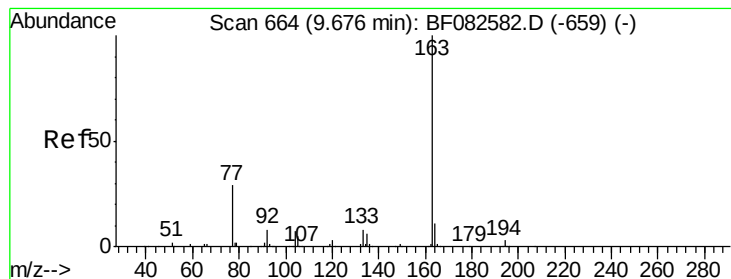

#49

Dimethylphthalate

Concen: 17.12 ng

RT: 9.62 min Scan# 659

Delta R.T. -0.03 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47

Instrument :

BNA_F

ClientSampleId :

SB-05(18-20)


Tot Ion:163 Resp: 562257

Ion Ratio Lower Upper

163 100

194 3.3 2.6 4.0




164 10.8 8.7 13.1

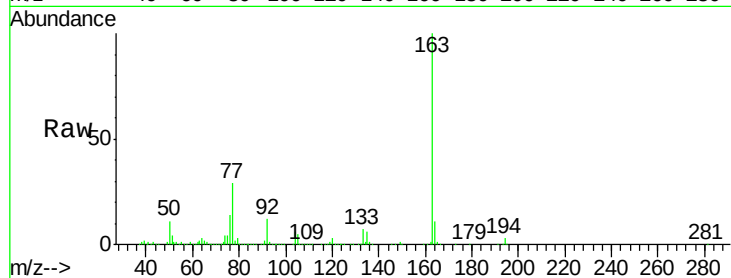

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

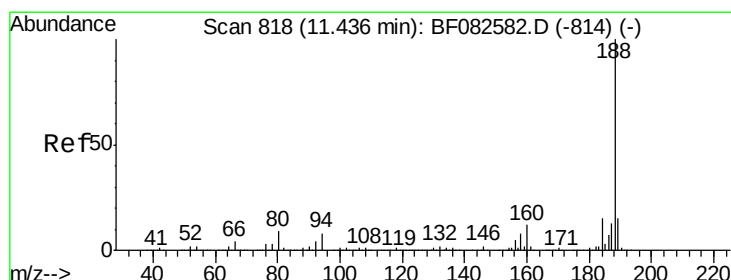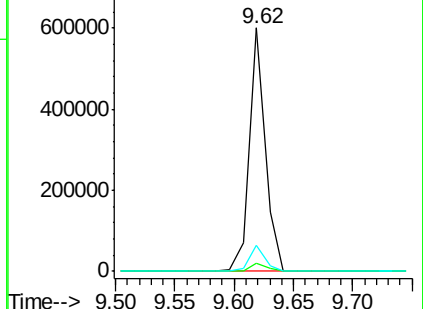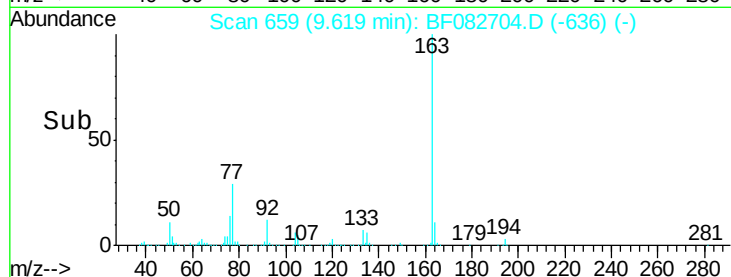

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.39 min Scan# 814

Delta R.T. -0.02 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47


Tgt Ion:188 Resp: 714227

Ion Ratio Lower Upper

188 100

94 4.7 6.1 9.1#



80 4.9 7.0 10.6#

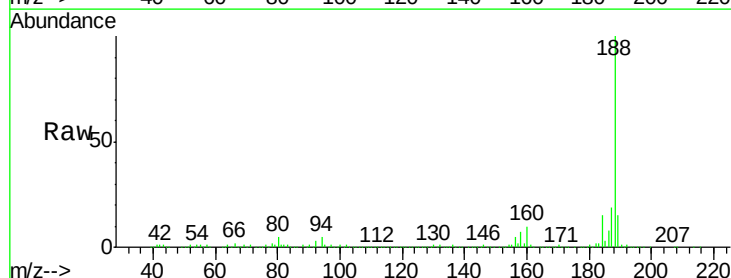


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

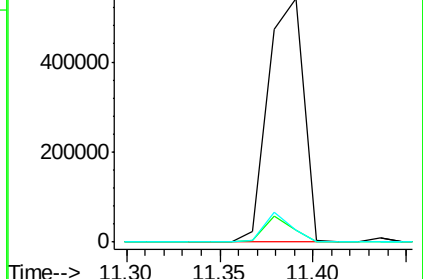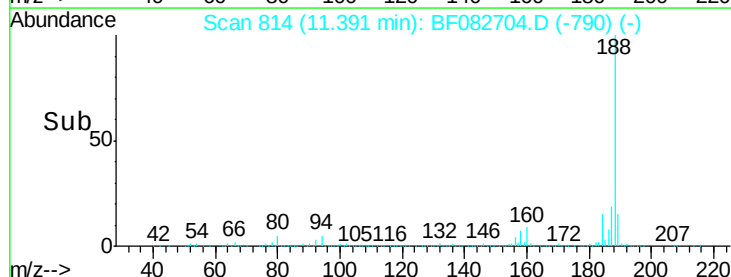

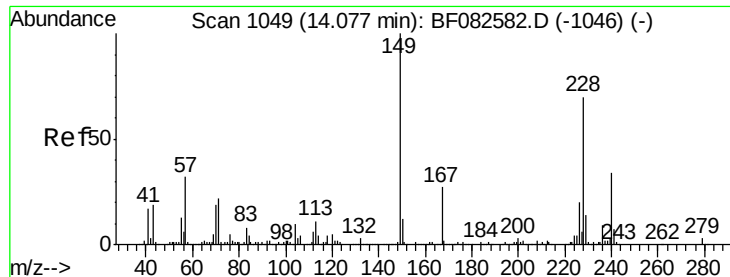

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.03 min Scan# 1045

Delta R.T. -0.02 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47

Instrument :

BNA_F

ClientSampleId :

SB-05(18-20)


Tot Ion:240 Resp: 693293

Ion Ratio Lower Upper

240 100

120 5.0 10.9 16.3#




236 26.1 21.6 32.4

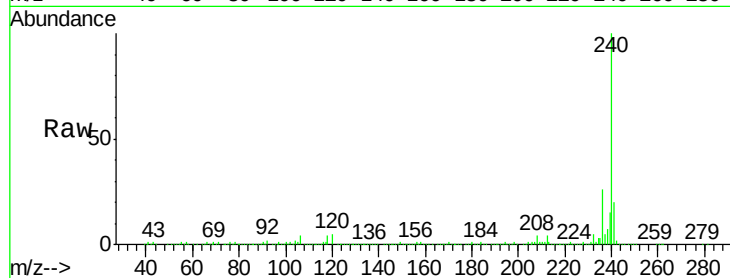

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

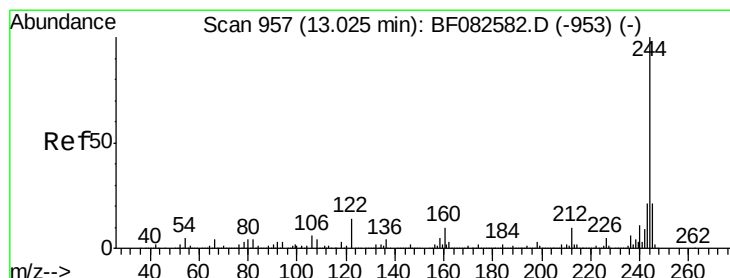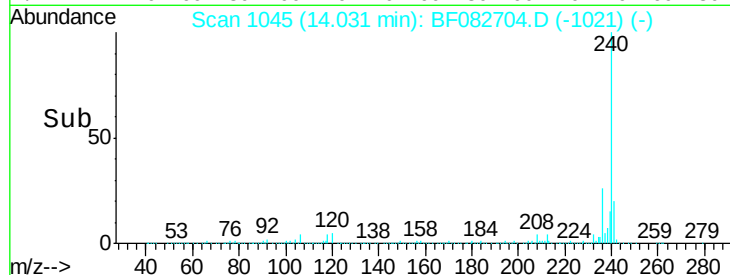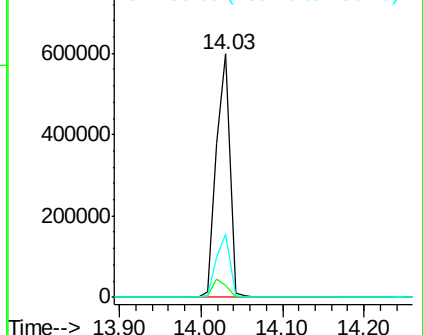

#78

Terphenyl-d14

Concen: 67.90 ng

RT: 12.98 min Scan# 953

Delta R.T. -0.02 min

Lab File: BF082704.D

Acq: 4 Nov 2015 16:47


Tgt Ion:244 Resp: 2151180

Ion Ratio Lower Upper

244 100

212 8.4 7.6 11.4



122 8.7 11.3 16.9#

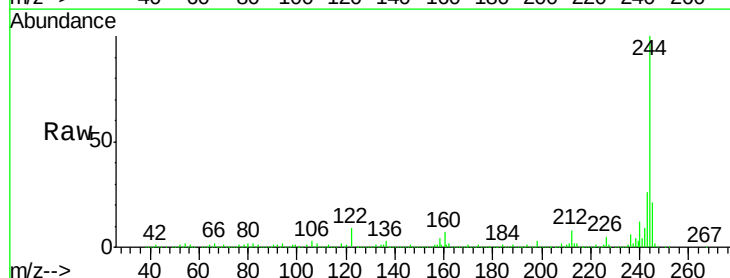


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

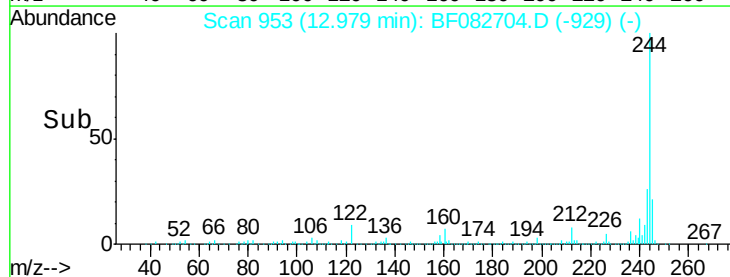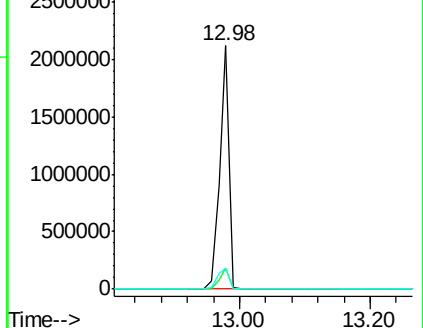


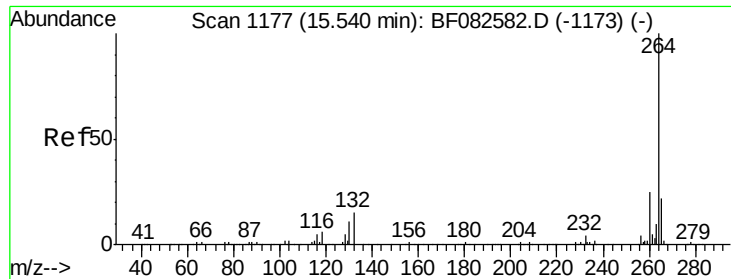

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.48 min Scan# 1172
Delta R.T. -0.02 min
Lab File: BF082704.D
Acq: 4 Nov 2015 16:47

Instrument :
BNA_F
ClientSampleId :
SB-05(18-20)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.8	29.6
265	21.6	17.4	26.0

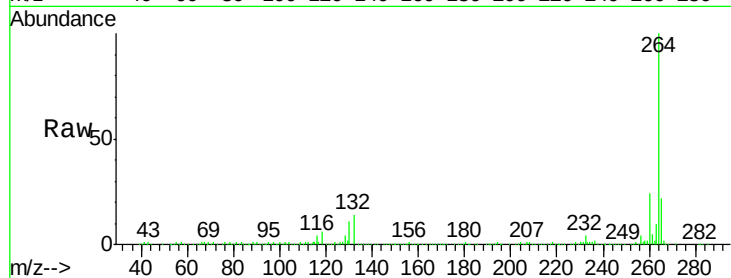

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

