


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110515\
 Data File : BF082694.D
 Acq On : 4 Nov 2015 11:57
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 03 12:27:47 2015

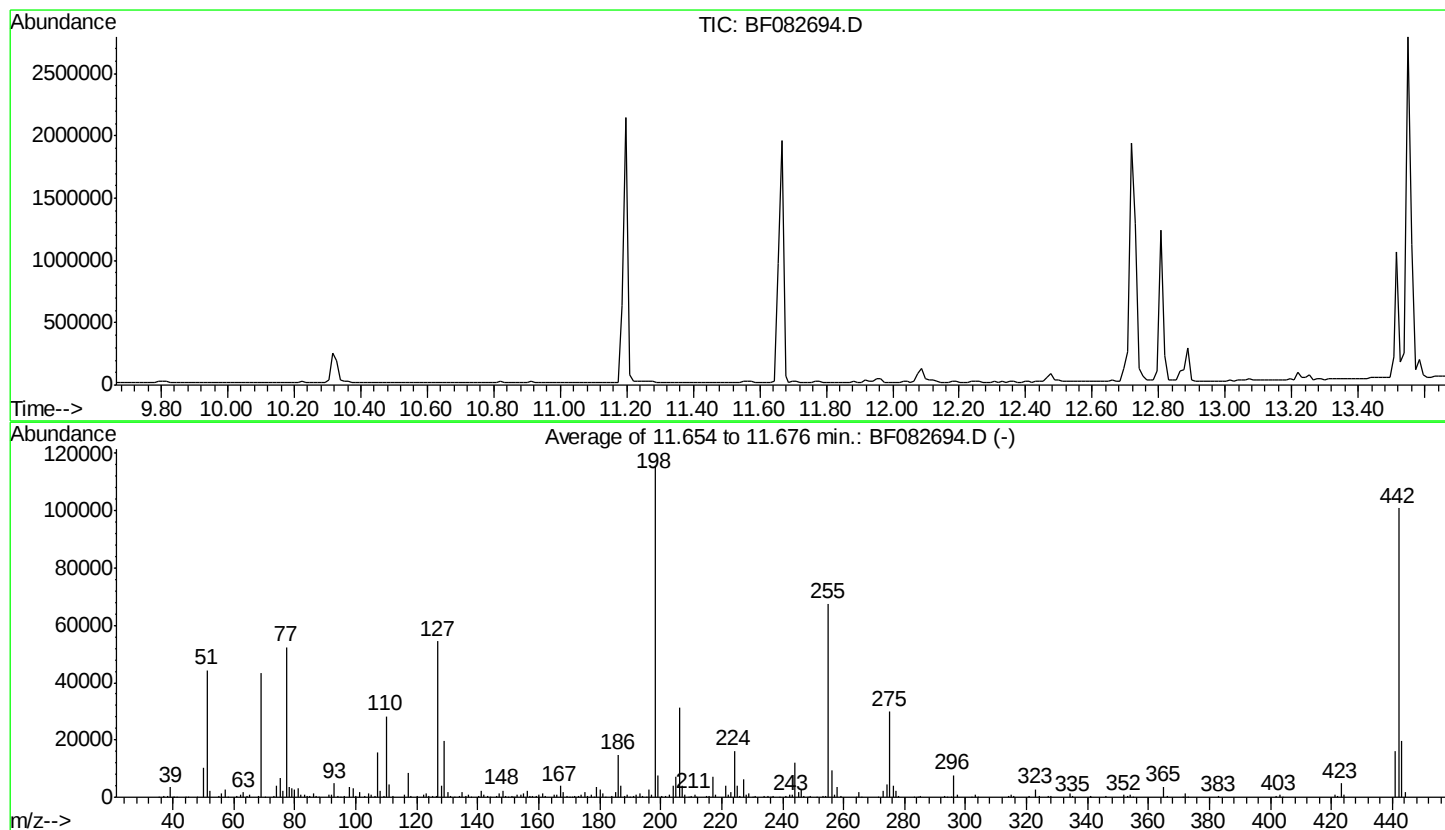

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	44298	PASS
68	69	0.00	2	1.6	681	PASS
69	198	0.00	100	37.5	43462	PASS
70	69	0.00	2	0.3	131	PASS
127	198	10	80	47.1	54502	PASS
197	198	0.00	2	0.9	1004	PASS
198	198	100	100	100.0	115757	PASS
199	198	5	9	6.5	7538	PASS
275	198	10	60	25.7	29784	PASS
365	198	1	100	3.1	3586	PASS
441	442	0.01	24	16.0	16176	PASS
442	198	50	100	87.1	100875	PASS
443	442	15	24	19.7	19889	PASS