

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110517\
 Data File : BF100229.D
 Acq On : 5 Nov 2017 17:39
 Operator : SJ/JU
 Sample : I6275-09 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 2727

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	492	496	500	rBV2	4766	8699	1.35%	0.184%
2	5.451	570	572	582	rBV3	17456	49667	7.70%	1.053%
3	6.492	745	749	758	rBV2	14912	42636	6.61%	0.904%
4	6.557	758	760	777	rVB	126623	228978	35.48%	4.856%
5	6.763	792	795	806	rBV	464793	459017	71.13%	9.735%
6	6.922	818	822	841	rBV	200386	241654	37.45%	5.125%
7	7.310	885	888	892	rBV	17842	22398	3.47%	0.475%
8	7.345	892	894	914	rVB	92112	155046	24.03%	3.288%
9	7.769	963	966	967	rBV	8993	7742	1.20%	0.164%
10	7.939	989	995	998	rBV2	7913	7123	1.10%	0.151%
11	8.045	1010	1013	1027	rBV	638717	645301	100.00%	13.685%
12	9.116	1191	1195	1202	rBV	372092	347102	53.79%	7.361%
13	9.792	1307	1310	1320	rVB	602378	577194	89.45%	12.241%
14	10.598	1444	1447	1455	rBV	118692	119393	18.50%	2.532%
15	11.216	1549	1552	1557	rBV5	4049	6837	1.06%	0.145%
16	11.286	1561	1564	1571	rBV	528229	467884	72.51%	9.923%
17	11.410	1582	1585	1589	rBV3	5476	8298	1.29%	0.176%
18	11.804	1649	1652	1655	rBV5	7066	7641	1.18%	0.162%
19	12.863	1829	1832	1838	rVB	312457	249823	38.71%	5.298%
20	13.268	1896	1901	1904	rBV7	8482	14561	2.26%	0.309%
21	13.710	1973	1976	1979	rVB3	16372	16466	2.55%	0.349%
22	13.939	2011	2015	2020	rBV	517182	507597	78.66%	10.765%
23	14.386	2089	2091	2092	rBV2	8612	6747	1.05%	0.143%
24	14.727	2146	2149	2156	rVB4	17611	33294	5.16%	0.706%
25	15.339	2251	2253	2258	rVB5	12584	14845	2.30%	0.315%
26	15.398	2258	2263	2271	rBV	334181	457410	70.88%	9.701%
27	15.745	2320	2322	2326	rVB5	11127	11966	1.85%	0.254%


Sum of corrected areas: 4715319

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110517\
Data File : BF100229.D
Acq On : 5 Nov 2017 17:39
Operator : SJ/JU
Sample : I6275-09 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2727

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

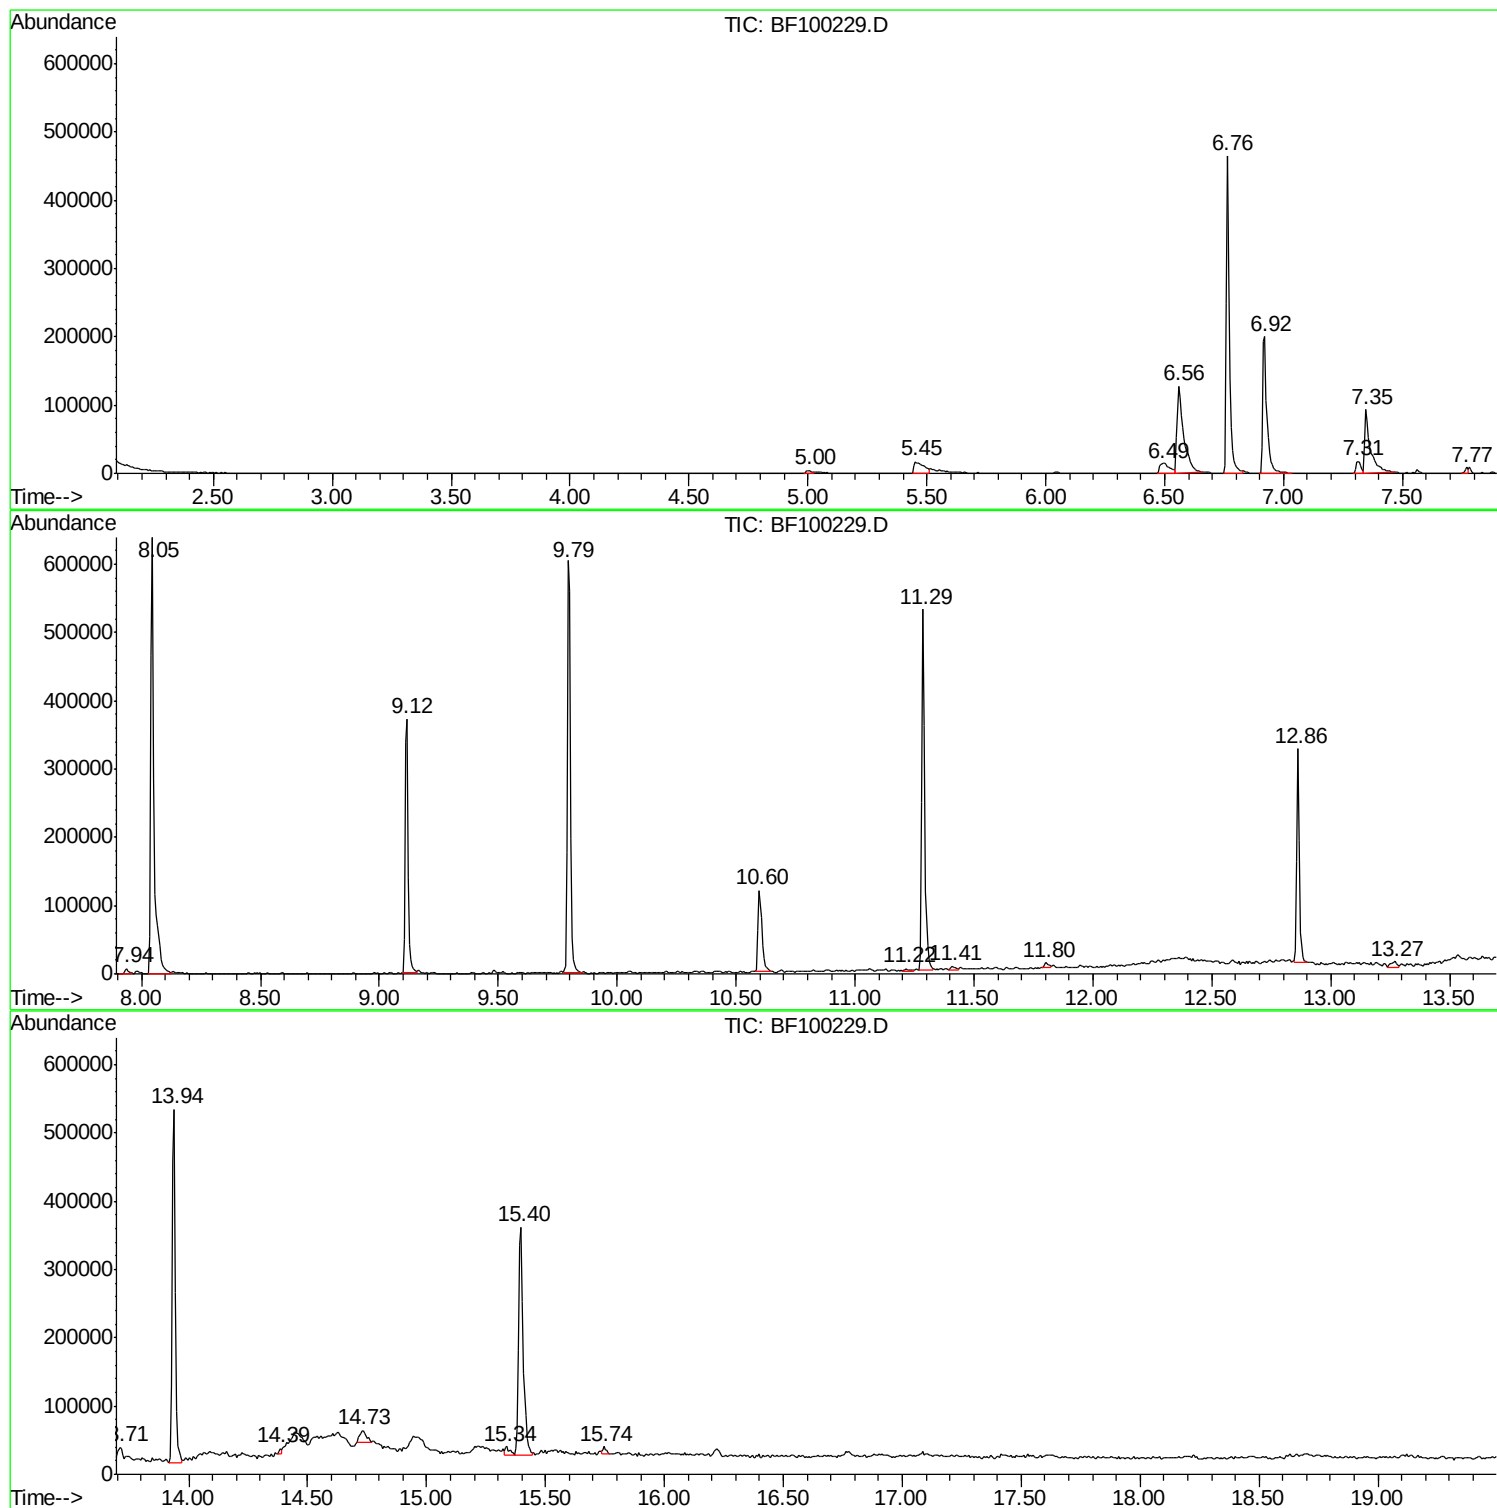

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF110517\
Data File : BF100229.D
Acq On : 5 Nov 2017 17:39
Operator : SJ/JU
Sample : I6275-09 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2727










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	9.98 ng	228978	1,4-Dichlorobenzene-d4	6.76

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	35
2	(E)-3-Chloro-2-methyl-2-pentenal			132	C6H9ClO	031357-76-3	25
3	5-Aminoindole			132	C8H8N2	005192-03-0	12
4	Amphetaminil			250	C17H18N2	017590-01-1	12
5	1-Methylpyrrolo[1,2-a]pyrazine			132	C8H8N2	064608-59-9	9

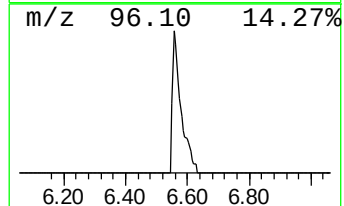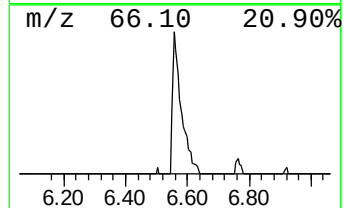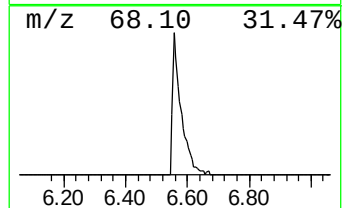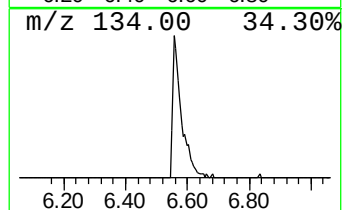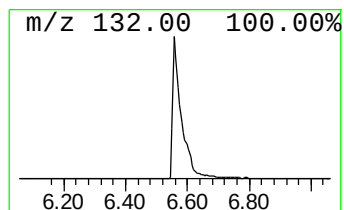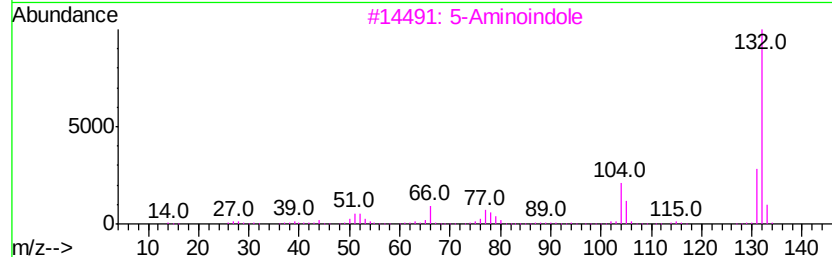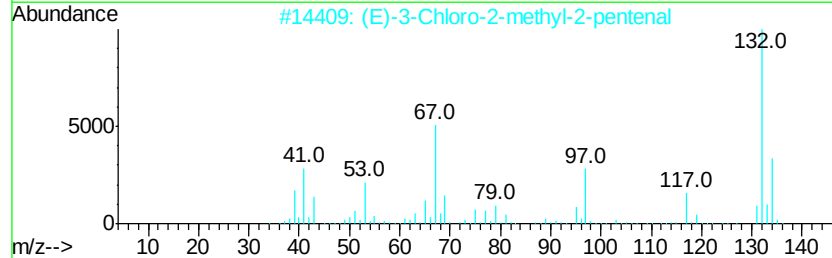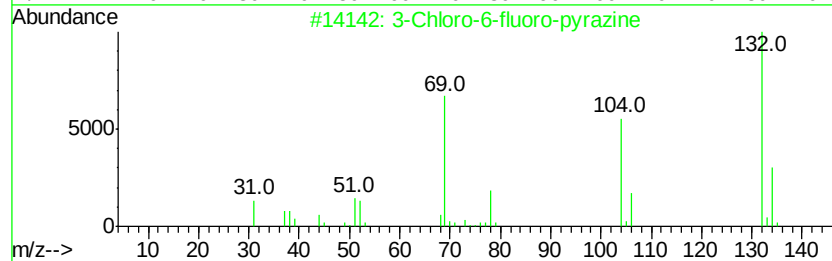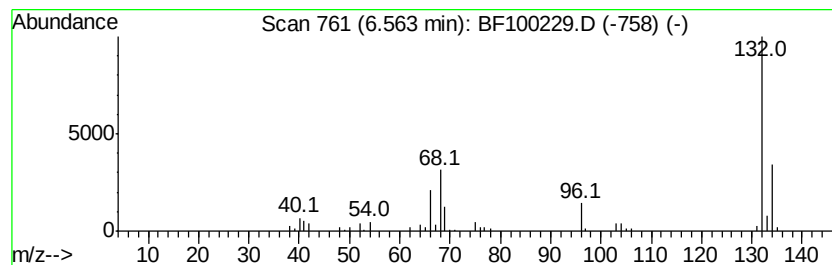

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF110517\
Data File : BF100229.D
Acq On : 5 Nov 2017 17:39
Operator : SJ/JU
Sample : I6275-09 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2727

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	10.0	ng	228978	1	6.76	459017	20.0