


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF110517\
 Data File : BF100215.D
 Acq On : 5 Nov 2017 10:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 03 15:46:10 2017

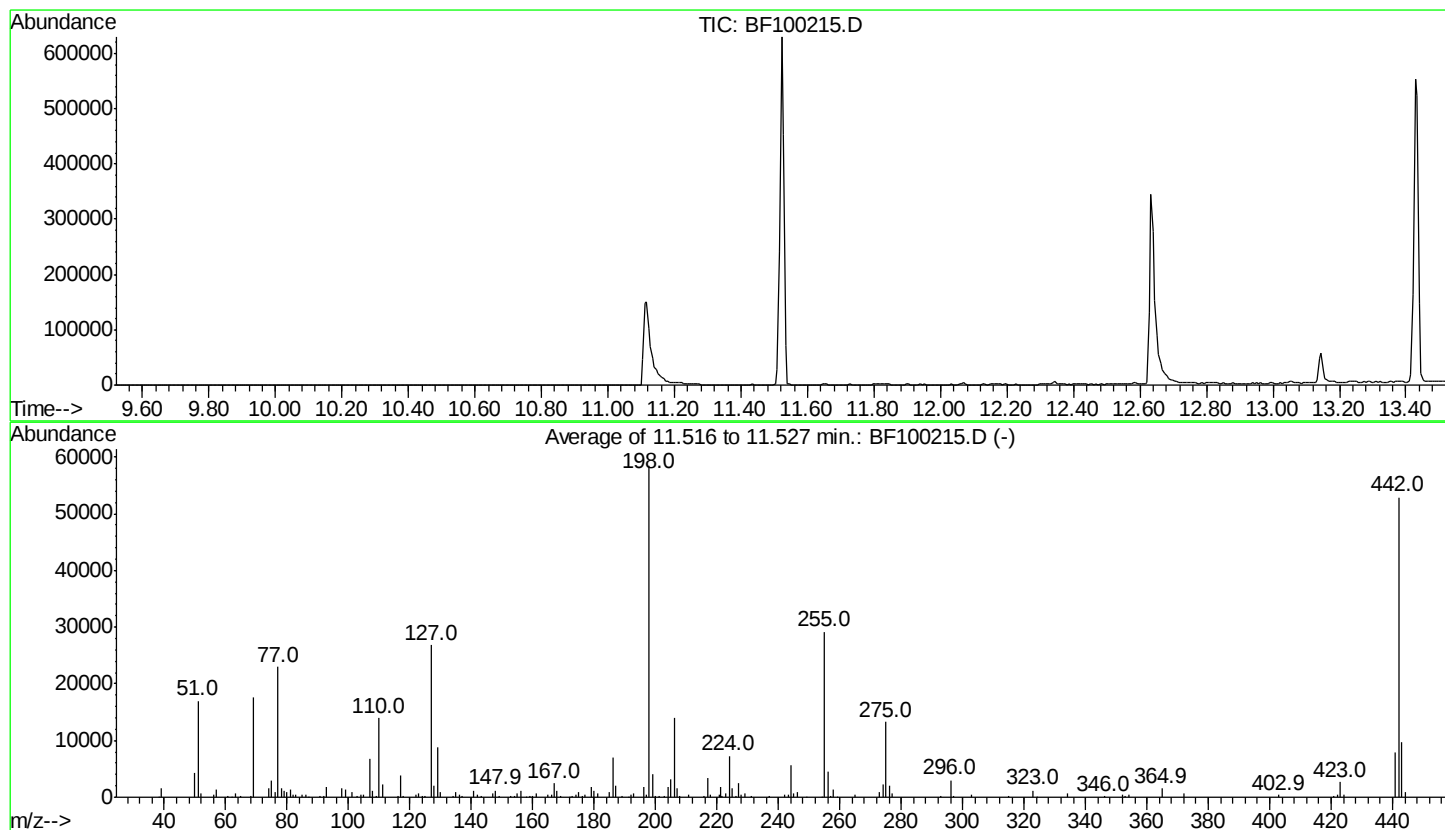

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	17015	PASS
68	69	0.00	2	1.1	186	PASS
69	198	0.00	100	30.3	17692	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	26848	PASS
197	198	0.00	2	0.9	517	PASS
198	198	100	100	100.0	58472	PASS
199	198	5	9	6.8	3963	PASS
275	198	10	60	22.8	13307	PASS
365	198	1	100	2.6	1512	PASS
441	443	0.01	100	81.6	7916	PASS
442	198	50	100	90.4	52839	PASS
443	442	15	24	18.4	9704	PASS