

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110615\
 Data File : BF082740.D
 Acq On : 5 Nov 2015 20:29
 Operator : UM/IZ
 Sample : G4261-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-5

Quant Time: Nov 06 03:13:14 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 03 12:27:47 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	78992	20.00	ng	-0.01
21) Naphthalene-d8	8.14	136	267873	20.00	ng	-0.02
38) Acenaphthene-d10	9.90	164	143125	20.00	ng	-0.02
63) Phenanthrene-d10	11.38	188	223362	20.00	ng	-0.03
75) Chrysene-d12	14.02	240	164601	20.00	ng	-0.03
86) Perylene-d12	15.45	264	163594	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	999991	190.67	ng	0.00
7) Phenol-d6	6.50	99	1434625	205.90	ng	-0.01
23) Nitrobenzene-d5	7.42	82	873832	133.21	ng	-0.02
41) 2,4,6-Tribromophenol	10.69	330	318533	203.36	ng	-0.02
44) 2-Fluorobiphenyl	9.23	172	1524417	151.22	ng	-0.02
78) Terphenyl-d14	12.97	244	1101701	146.48	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.62	163	304818	26.08	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF110615\
Data File : BF082740.D
Acq On : 5 Nov 2015 20:29
Operator : UM/IZ
Sample : G4261-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-5

Quant Time: Nov 06 03:13:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF103015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 03 12:27:47 2015
Response via : Initial Calibration

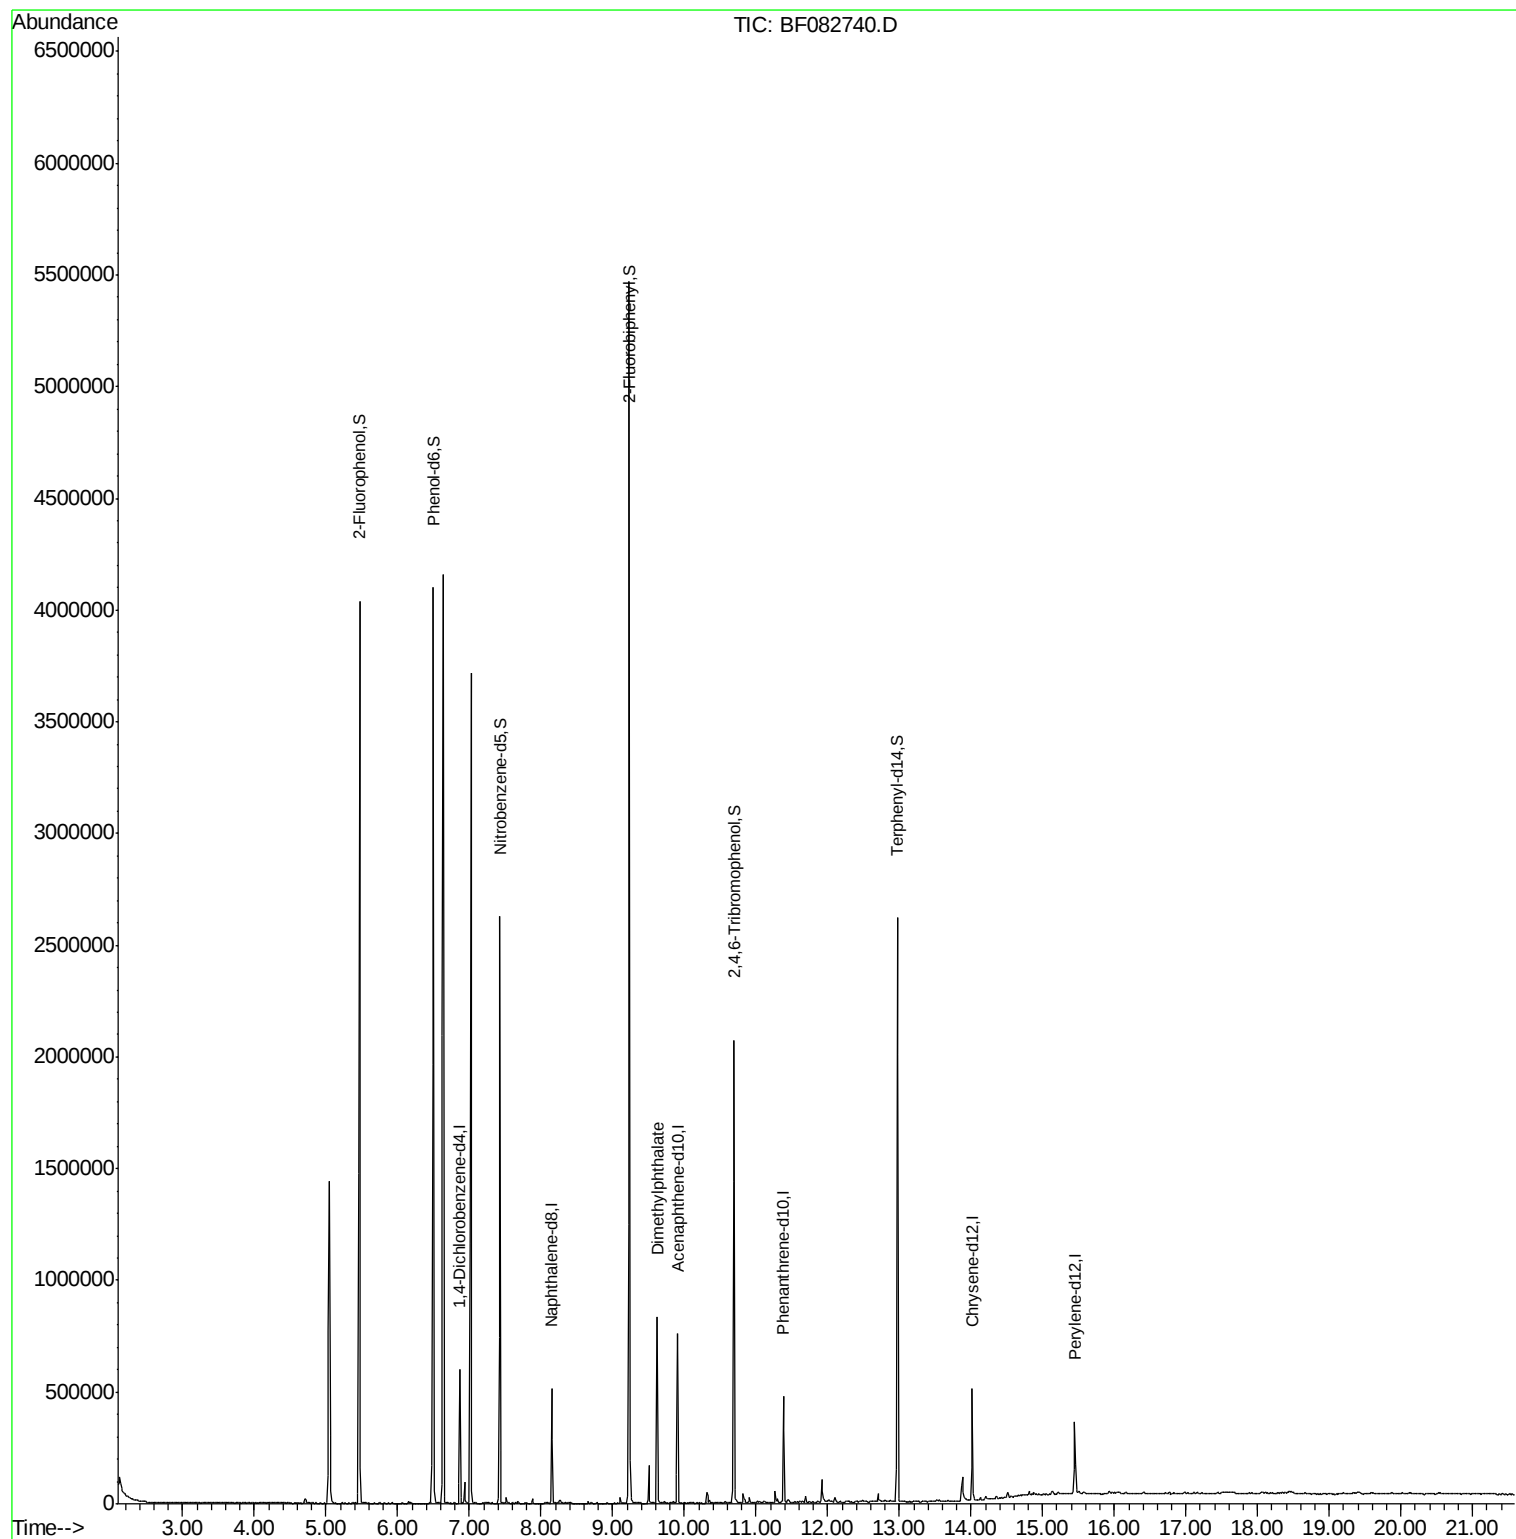

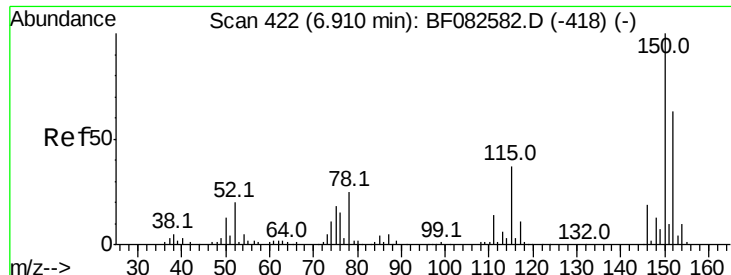

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 418

Delta R.T. -0.01 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29

Instrument :

BNA_F

ClientSampleId :

SB-5


Tot Ion:152 Resp: 78992

Ion Ratio Lower Upper

152 100

150 155.0 127.0 190.4




115 62.7 47.0 70.6

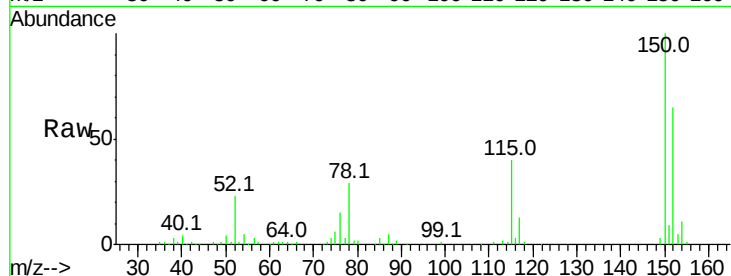

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

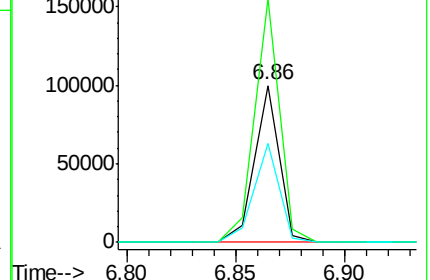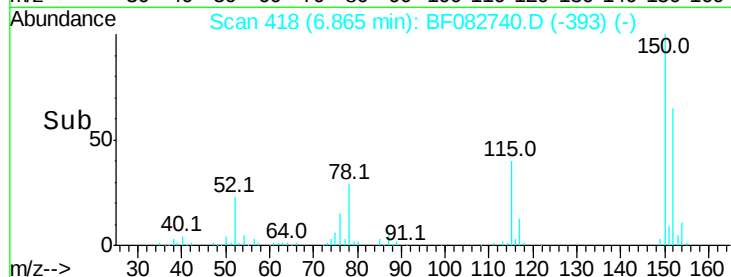

#5

2-Fluorophenol

Concen: 190.67 ng

RT: 5.47 min Scan# 296

Delta R.T. 0.00 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29


Tgt Ion:112 Resp: 999991

Ion Ratio Lower Upper

112 100

64 68.5 48.9 73.3



63 37.1 28.1 42.1




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

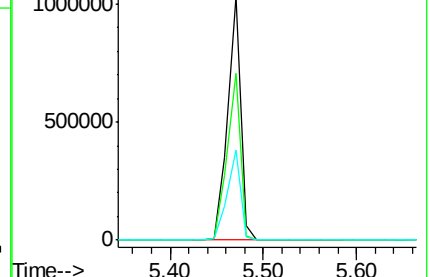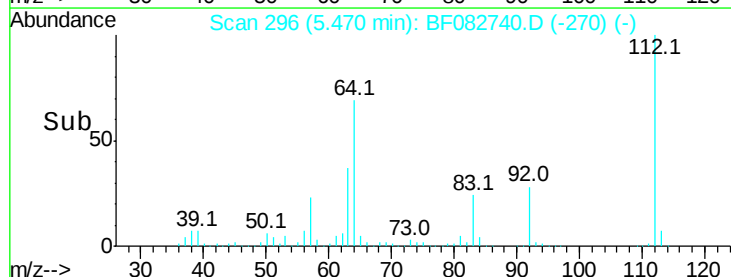

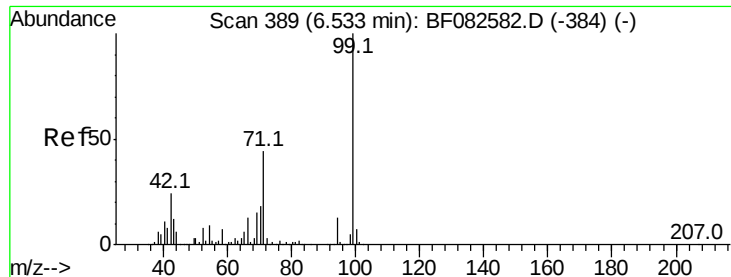

#7

Phenol-d6

Concen: 205.90 ng

RT: 6.50 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29

Instrument :

BNA_F

ClientSampleId :

SB-5


Tot Ion: 99 Resp: 1434625

Ion Ratio Lower Upper

99 100

42 20.5 19.2 28.8




71 39.9 35.0 52.4

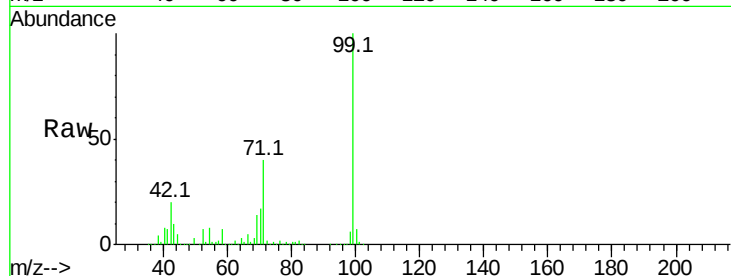

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

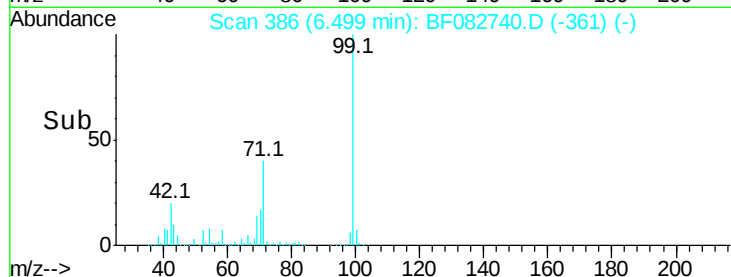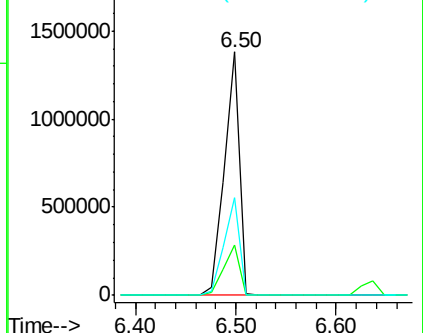

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 530

Delta R.T. -0.02 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29

Tgt Ion: 136 Resp: 267873


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 11.0 9.1 13.7

68 6.7 4.8 7.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

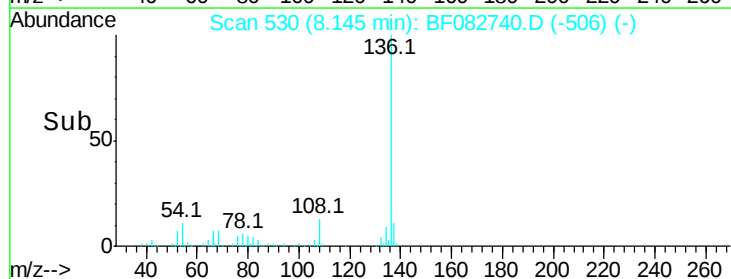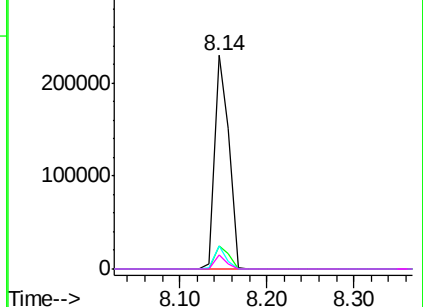


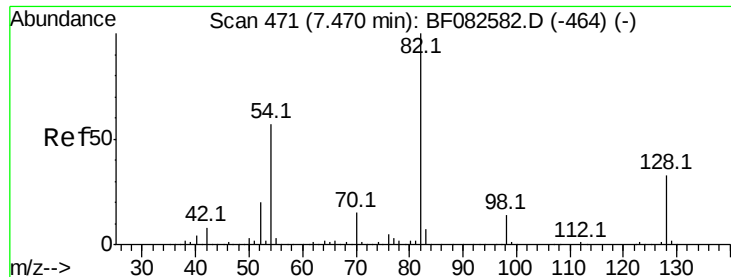




#23
Nitrobenzene-d5
Concen: 133.21 ng
RT: 7.42 min Scan# 467
Delta R.T. -0.02 min
Lab File: BF082740.D
Acq: 5 Nov 2015 20:29

Instrument :
BNA_F
ClientSampleID :
SB-5

Tot Ion: 82 Resp: 873832
Ion Ratio Lower Upper
82 100
128 35.6 26.8 40.2
54 53.8 45.7 68.5

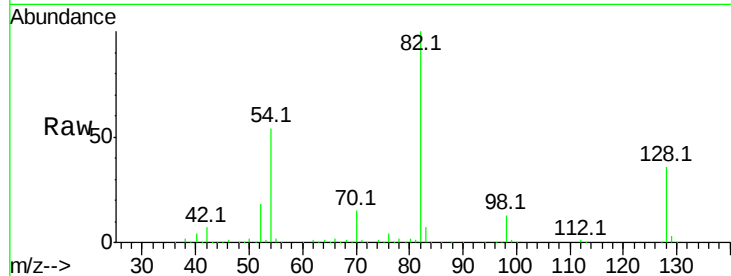


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

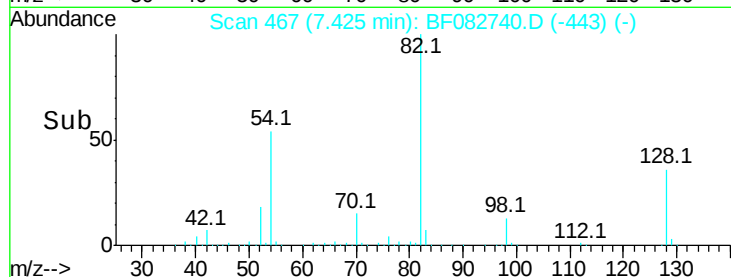
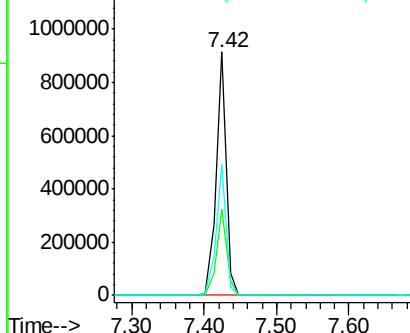



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.90 min Scan# 684
Delta R.T. -0.02 min
Lab File: BF082740.D
Acq: 5 Nov 2015 20:29

Tgt Ion:164 Resp: 143125
Ion Ratio Lower Upper
164 100
162 102.0 84.9 127.3
160 43.3 37.5 56.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

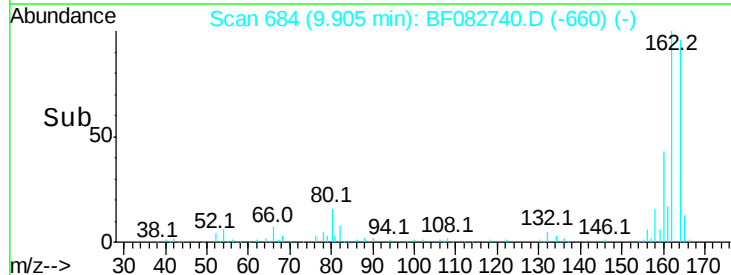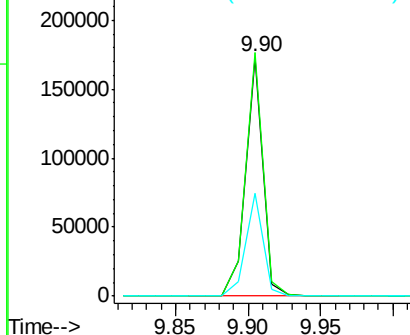


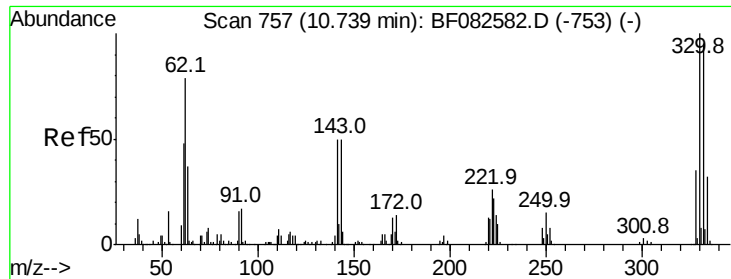




#41
 2,4,6-Tribromophenol
 Concen: 203.36 ng
 RT: 10.69 min Scan# 753
 Delta R.T. -0.02 min
 Lab File: BF082740.D
 Acq: 5 Nov 2015 20:29

Instrument :
 BNA_F
 ClientSampleId :
 SB-5

Tot Ion:330 Resp: 318533
 Ion Ratio Lower Upper
 330 100
 332 94.6 76.6 114.8
 141 35.3 41.2 61.8#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

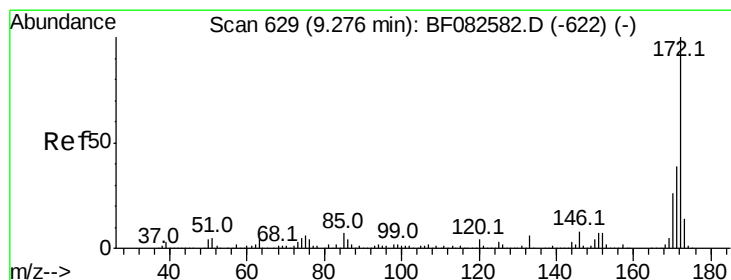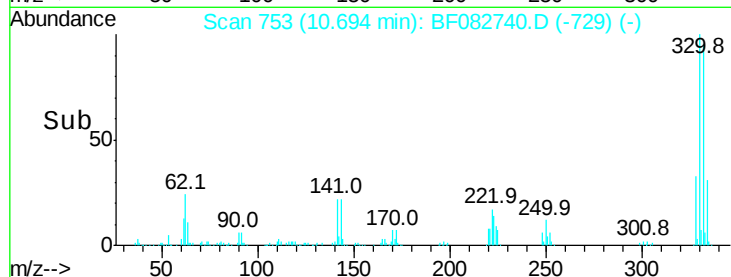
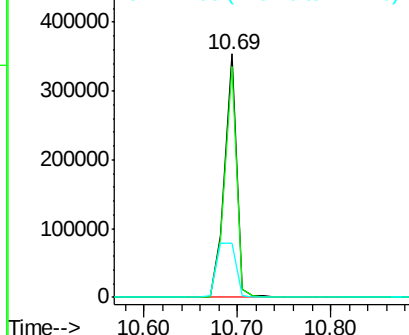



#44
 2-Fluorobiphenyl
 Concen: 151.22 ng
 RT: 9.23 min Scan# 625
 Delta R.T. -0.02 min
 Lab File: BF082740.D
 Acq: 5 Nov 2015 20:29

Tgt Ion:172 Resp: 1524417
 Ion Ratio Lower Upper
 172 100
 171 37.1 30.8 46.2
 170 25.8 21.2 31.8

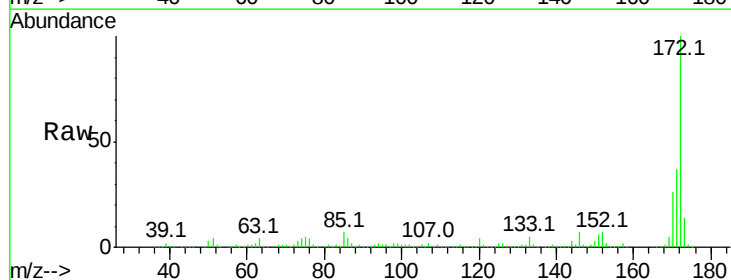

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

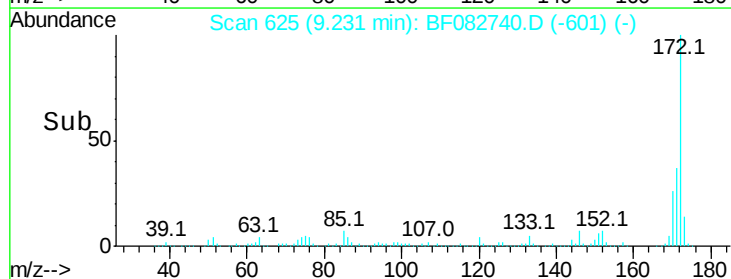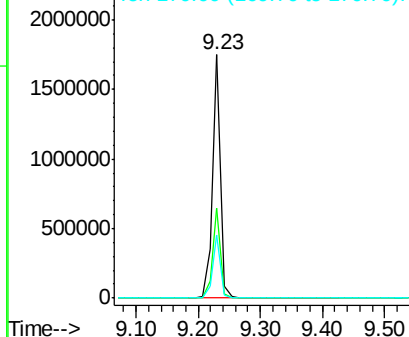

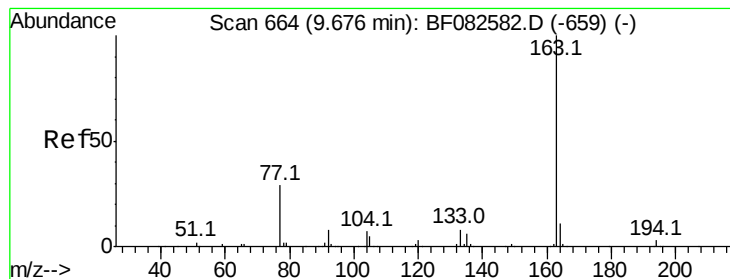

#49

Dimethylphthalate

Concen: 26.08 ng

RT: 9.62 min Scan# 659

Delta R.T. -0.03 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29

Instrument :

BNA_F

ClientSampleId :

SB-5


Tot Ion:163 Resp: 304818

Ion Ratio Lower Upper

163 100

194 3.1 2.6 4.0




164 10.2 8.7 13.1

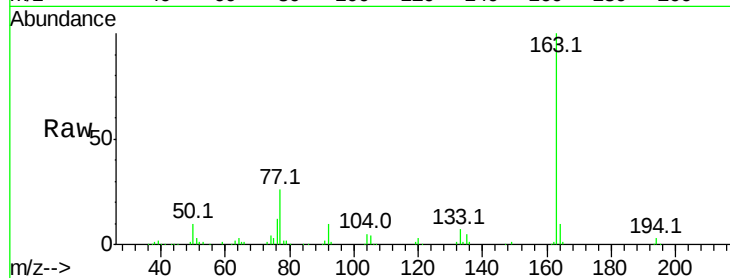

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

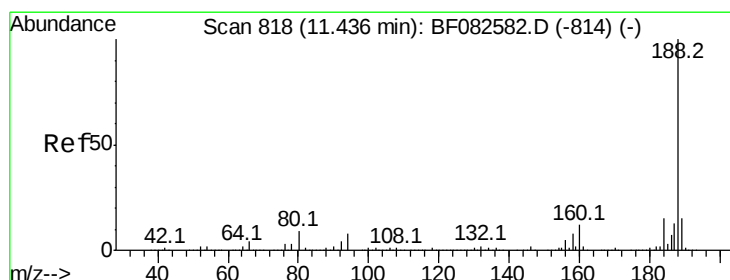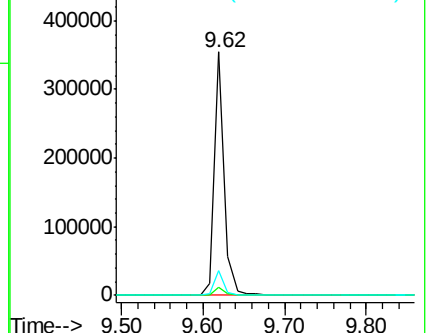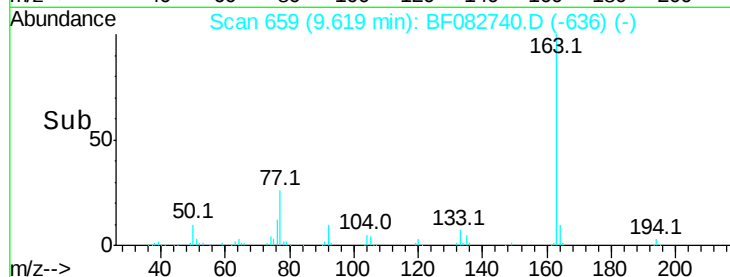

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.38 min Scan# 813

Delta R.T. -0.03 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29


Tgt Ion:188 Resp: 223362

Ion Ratio Lower Upper

188 100

94 12.5 6.1 9.1#



80 13.2 7.0 10.6#

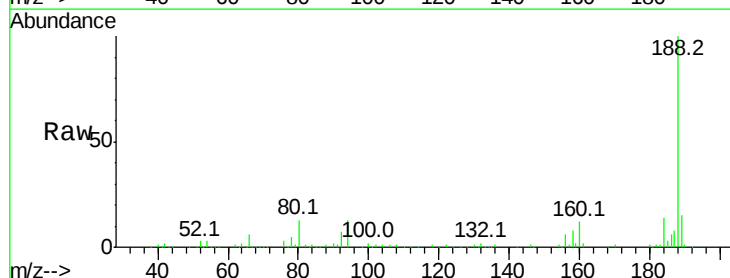


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

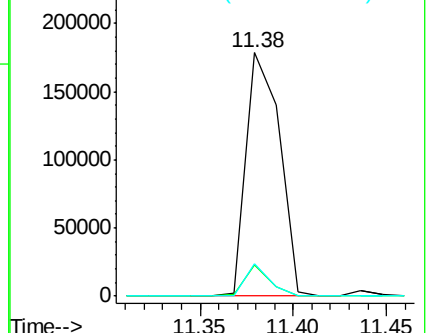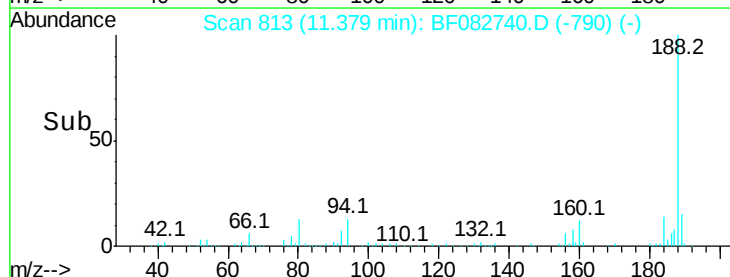

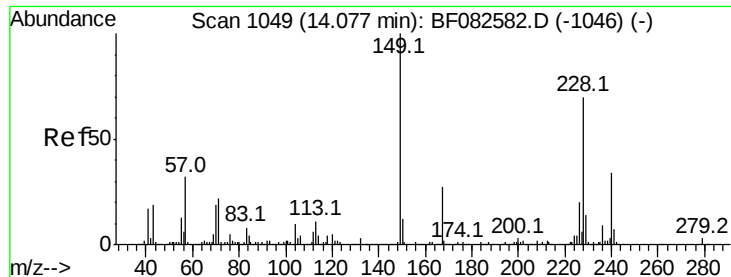

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.02 min Scan# 1044

Delta R.T. -0.03 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29

Instrument :

BNA_F

ClientSampleID :

SB-5


Tot Ion:240 Resp: 164601

Ion Ratio Lower Upper

240 100

120 7.0 10.9 16.3#




236 25.5 21.6 32.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

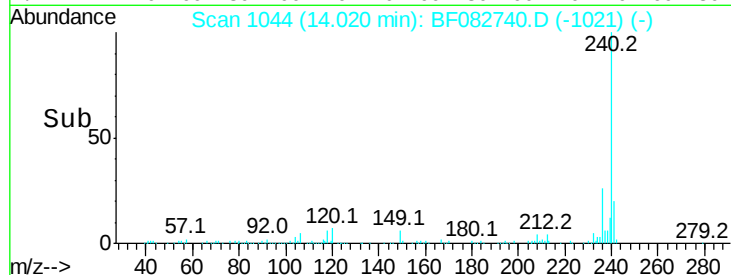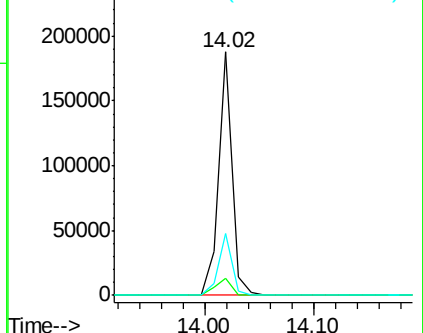

#78

Terphenyl-d14

Concen: 146.48 ng

RT: 12.97 min Scan# 952

Delta R.T. -0.03 min

Lab File: BF082740.D

Acq: 5 Nov 2015 20:29


Tgt Ion:244 Resp: 1101701

Ion Ratio Lower Upper

244 100

212 8.3 7.6 11.4



122 14.2 11.3 16.9




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

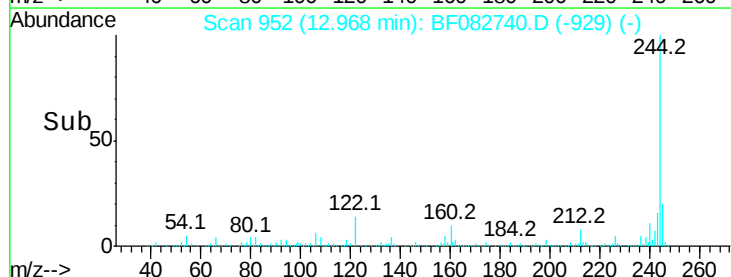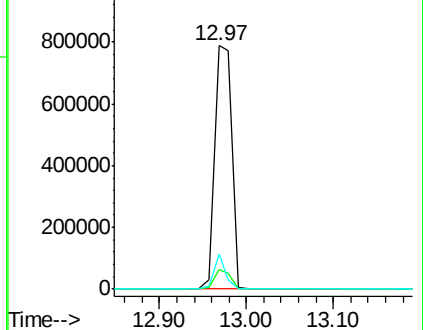


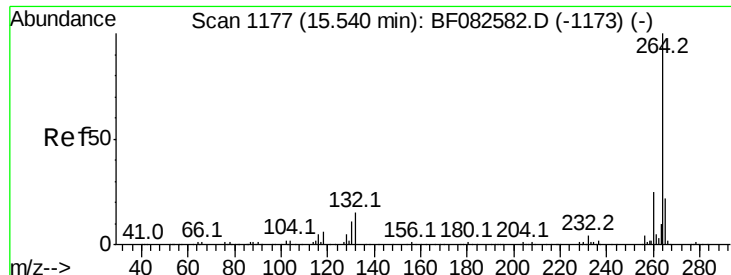

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.45 min Scan# 1169
 Delta R.T. -0.06 min
 Lab File: BF082740.D
 Acq: 5 Nov 2015 20:29

Instrument :
 BNA_F
 ClientSampleId :
 SB-5

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.6
265	20.7	17.4	26.0



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

