


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF110615\
 Data File : BF082741.D
 Acq On : 5 Nov 2015 23:40
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF103015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 03 12:27:47 2015

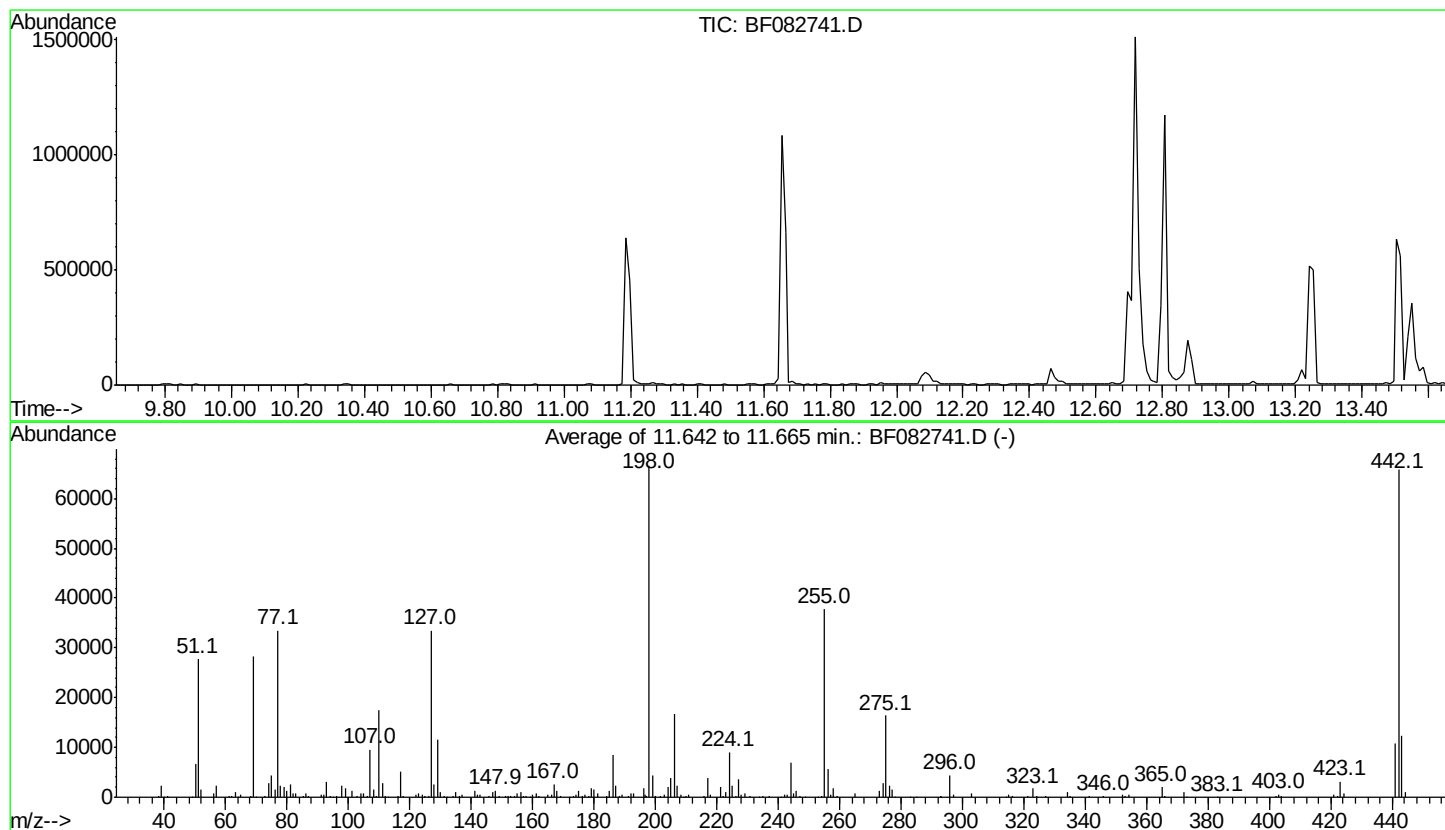

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	27819	PASS
68	69	0.00	2	1.2	353	PASS
69	198	0.00	100	42.6	28381	PASS
70	69	0.00	2	0.4	122	PASS
127	198	10	80	50.4	33544	PASS
197	198	0.00	2	0.6	396	PASS
198	198	100	100	100.0	66620	PASS
199	198	5	9	6.6	4389	PASS
275	198	10	60	24.7	16453	PASS
365	198	1	100	3.2	2131	PASS
441	442	0.01	24	16.4	10799	PASS
442	198	50	100	98.9	65858	PASS
443	442	15	24	18.9	12455	PASS