
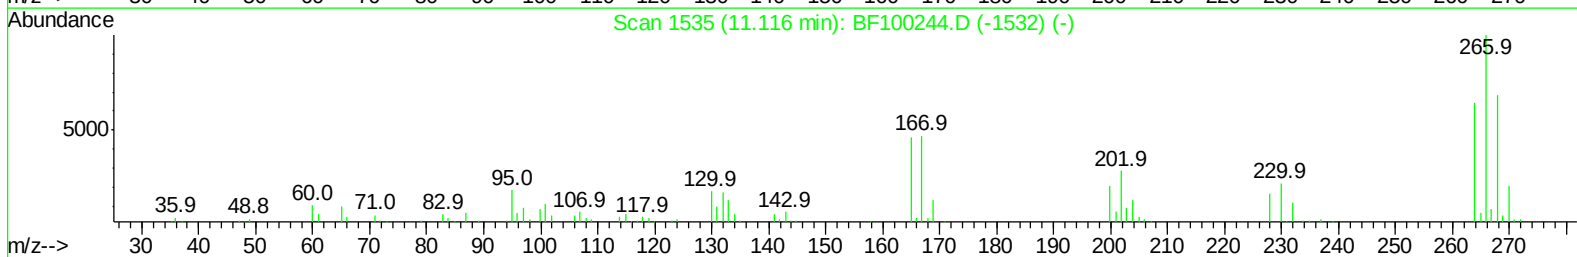
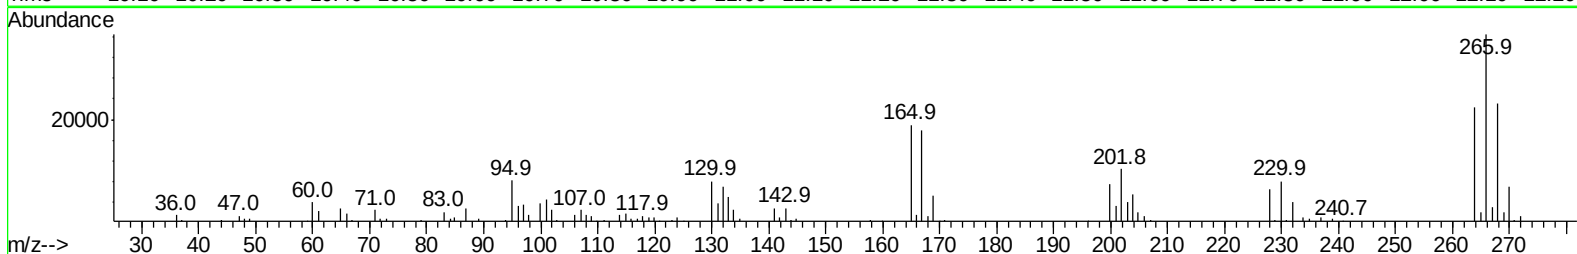


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF110617\
Data File : BF100243.D
Acq On : 6 Nov 2017 10:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 07:50:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:59:38 2017
Response via : Initial Calibration

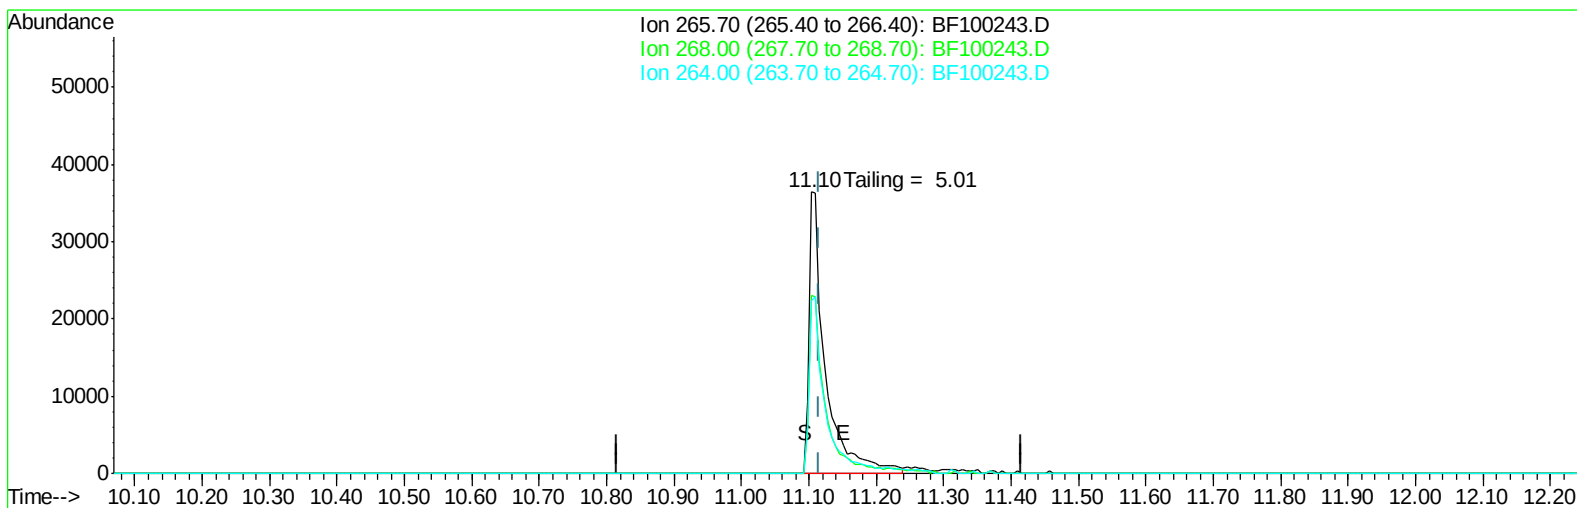

TIC: BF100243.D

(69) Pentachlorophenol (C)

11.104min (-0.012) 0.00ng

response 60622

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.20
264.00	61.90	61.32
0.00	0.00	0.00

